


SESAA Esterhazy Station - September 2023 Summary Report

Pollutants		Month Records		24-Hour Records				1-Hour Records			
Name	Conc. Unit	Avg. Conc.	Uptime	Maximum		SAAQS Standard	Exceed Days	Maximum		SAAQS Standard	Exceed Hours
				Conc.	Time			Conc.	Time		
NO	ppb	0.4	99.7%	2.3	Sep-21	-	-	18.0	Sep-21 07:00	-	-
NO ₂	ppb	0.3	99.7%	0.3	Sep-10	106	0	11.9	Sep-20 19:00	159	0
NO _x	ppb	0.5	99.7%	1.0	Sep-7	-	-	26.2	Sep-21 07:00	-	-
O ₃	ppb	24	99.7%	37	Sep-3	-	-	58	Sep-03 16:00	82	0
PM _{2.5}	ug/m3	17	99.7%	72	Sep-3	28	4	165	Sep-04 16:00	-	-


SAAQS: Saskatchewan Ambient Air Quality Standards



Monthly Update

- *All data has been slope, intercept, and baseline corrected. Data may change after validation process.
- *All compliance parameters were within the Saskatchewan Ambient Air Quality Standards with the exception of four 24-hour PM 2.5 exceedance associated with wildfire smoke in the area.
- *All compliance parameters were above 90% operational.
- *There are 8 hours of data for all parameters flagged as "power failure" due to intermittent power issues at the site.
- *Routine quarterly calibrations were completed on September 20, 2023

SESAA Esterhazy Station - September 2023 Summary Report

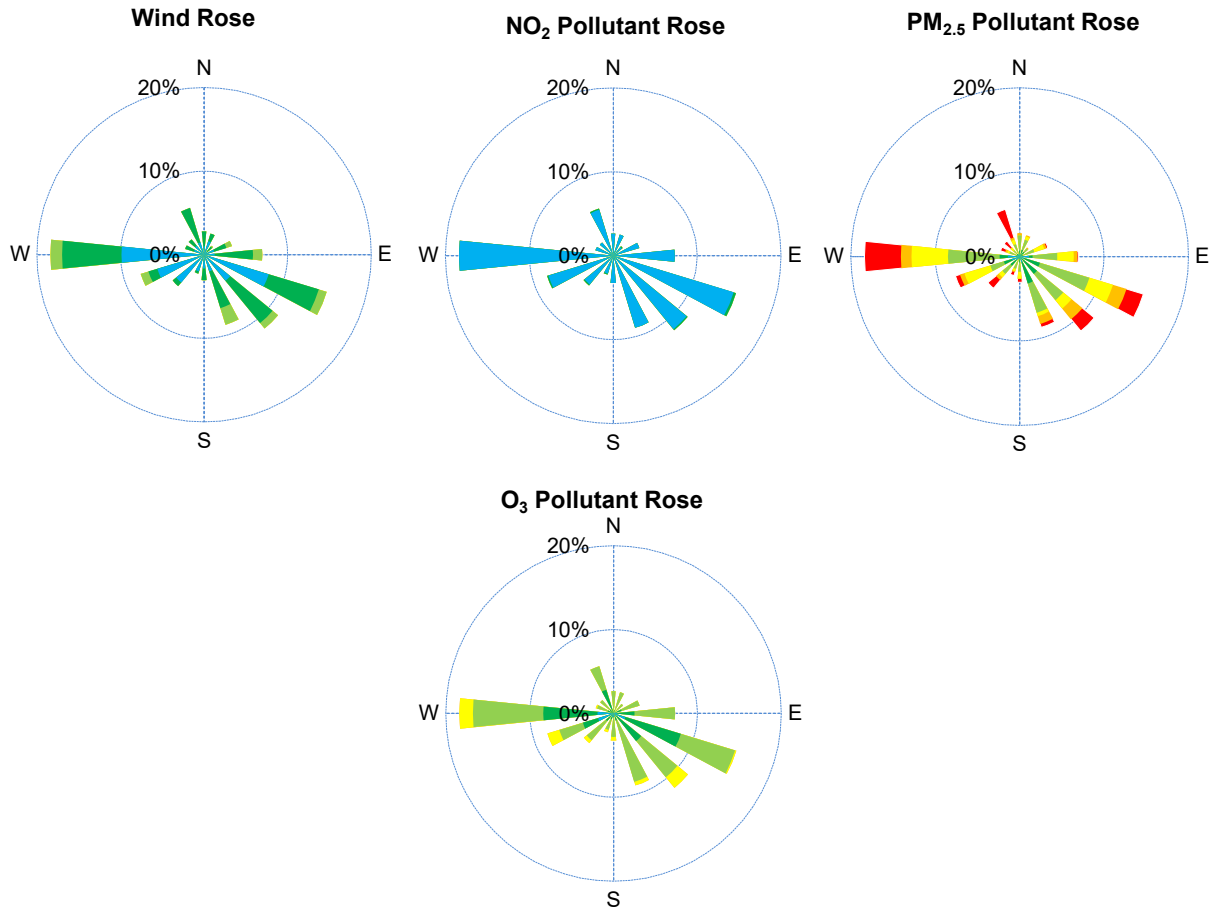



Parameters	Unit	Color Code for Wind Spd & Pollutant Conc. Class					
Wind Speed	m/s	0.3 ≤ WS < 1.4	1.4 ≤ WS < 3.1	3.1 ≤ WS < 7.8	7.8 ≤ WS < 10.8	10.8 ≤ WS < 13.6	WS ≥ 13.6
NO ₂	ppb	0 ≤ C < 5	5 ≤ C < 15	15 ≤ C < 30	30 ≤ C < 100	100 ≤ C < 212	C ≥ 212
PM _{2.5}	ug/m ³	0 ≤ C < 2	2 ≤ C < 4	4 ≤ C < 10	10 ≤ C < 20	20 ≤ C < 30	C ≥ 30
O ₃	ppb	0 ≤ C < 10	10 ≤ C < 20	20 ≤ C < 40	40 ≤ C < 60	60 ≤ C < 82	C ≥ 82

Exceedance Summary (24-Hour Average)											
24-hour Exceedance Information			Summary of Other Parameters During Exceedance								
Pollutant	Conc. ppb	Exceedance Date mmm-dd	WS m/s	WD deg	AQHI -	Rain mm	NO ppb	NO ₂ ppb	NO _x ppb	O ₃ ppb	PM _{2.5} ug/m ₃
PM _{2.5}	72	Sep-3	1.4	193	5	0.0	0.1	-	0.2	37	72
PM _{2.5}	71	Sep-4	1.7	278	5	0.2	0.2	-	-	29	71
PM _{2.5}	35	Sep-15	2.0	270	2	0.0	0.4	-	-	16	35
PM _{2.5}	32	Sep-19	1.6	295	3	0.0	-	-	-	28	32


SESAA Glen Ewen Station - September 2023 Summary Report

Pollutants		Month Records		24-Hour Records				1-Hour Records			
Name	Conc. Unit	Avg. Conc.	Uptime	Maximum		SAAQS Standard	Exceed Days	Maximum		SAAQS Standard	Exceed Hours
				Conc.	Time			Conc.	Time		
NO	ppb	0.3	99.9%	0.7	Sep-16	-	-	7.4	Sep-06 05:00	-	-
NO ₂	ppb	1.0	99.9%	2.0	Sep-19	106	0	5.6	Sep-09 21:00	159	0
NO _x	ppb	1.3	99.9%	2.3	Sep-19	-	-	12.3	Sep-06 05:00	-	-
SO ₂	ppb	0.2	100.0%	< 0.1	#N/A	48	0	7.1	Sep-18 11:00	172	0
O ₃	ppb	24	100.0%	36	Sep-3	-	-	61	Sep-03 16:00	82	0
H ₂ S	ppb	0.1	100.0%	0.3	Sep-3	3.6	0	9.0	Sep-16 03:00	11	0

SAAQS: Saskatchewan Ambient Air Quality Standards

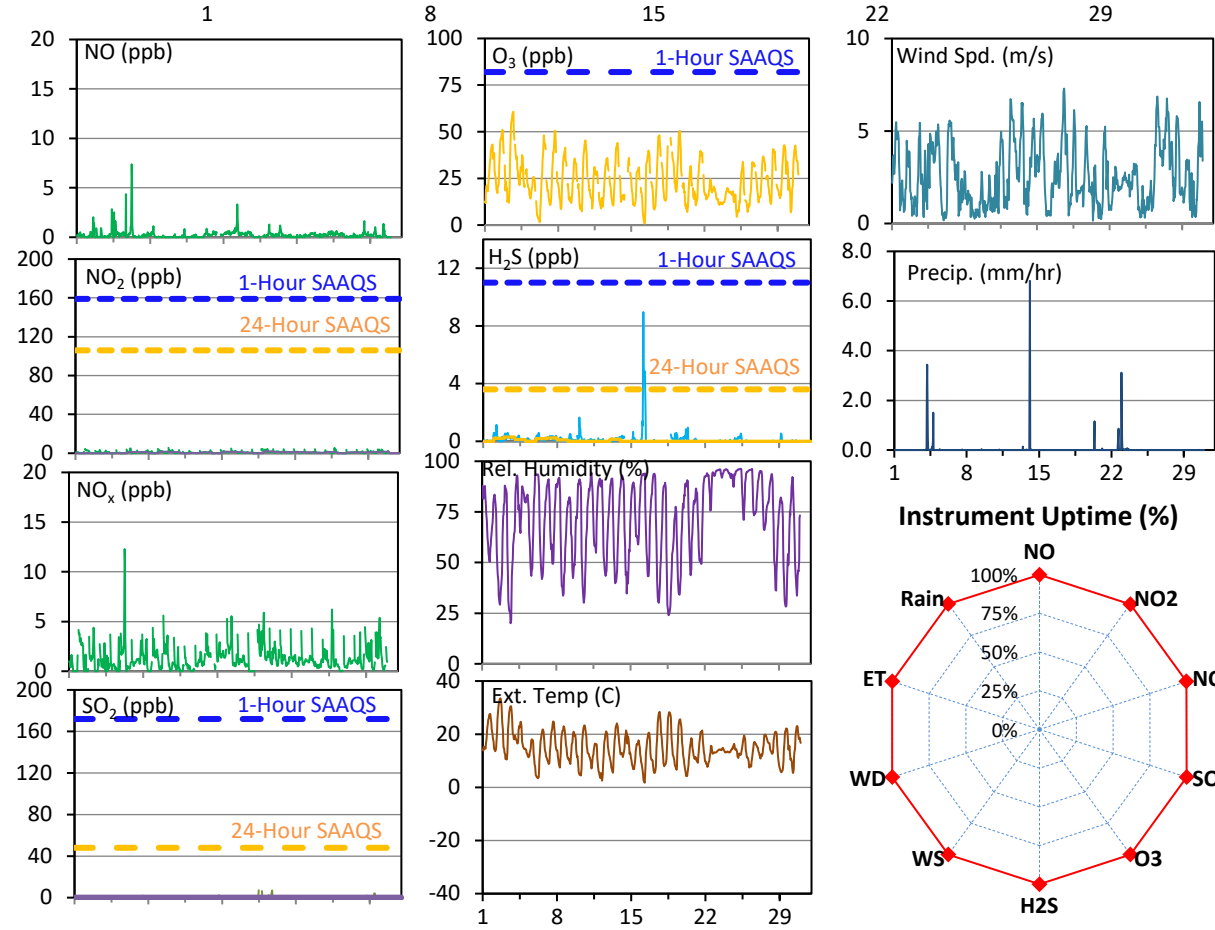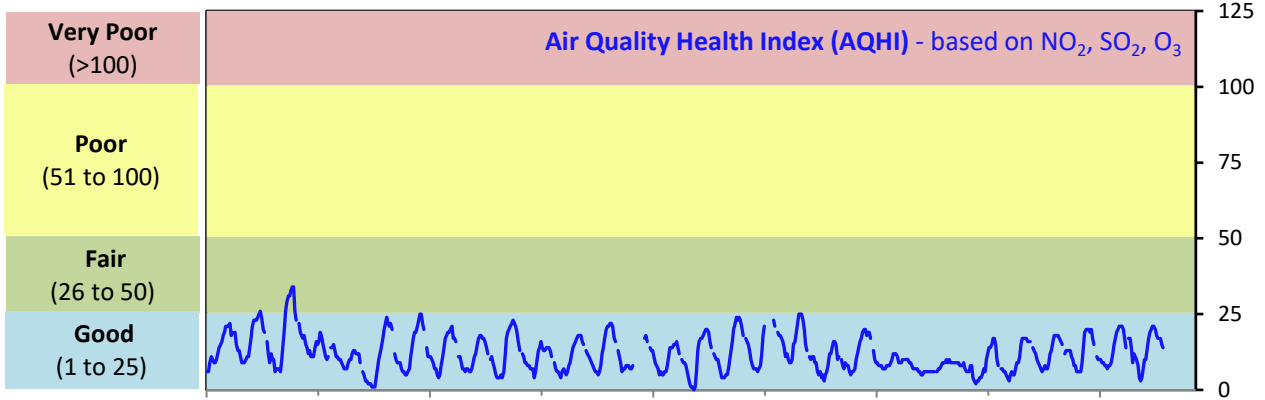

SESAA Glen Ewen Station - September 2023 Summary Report

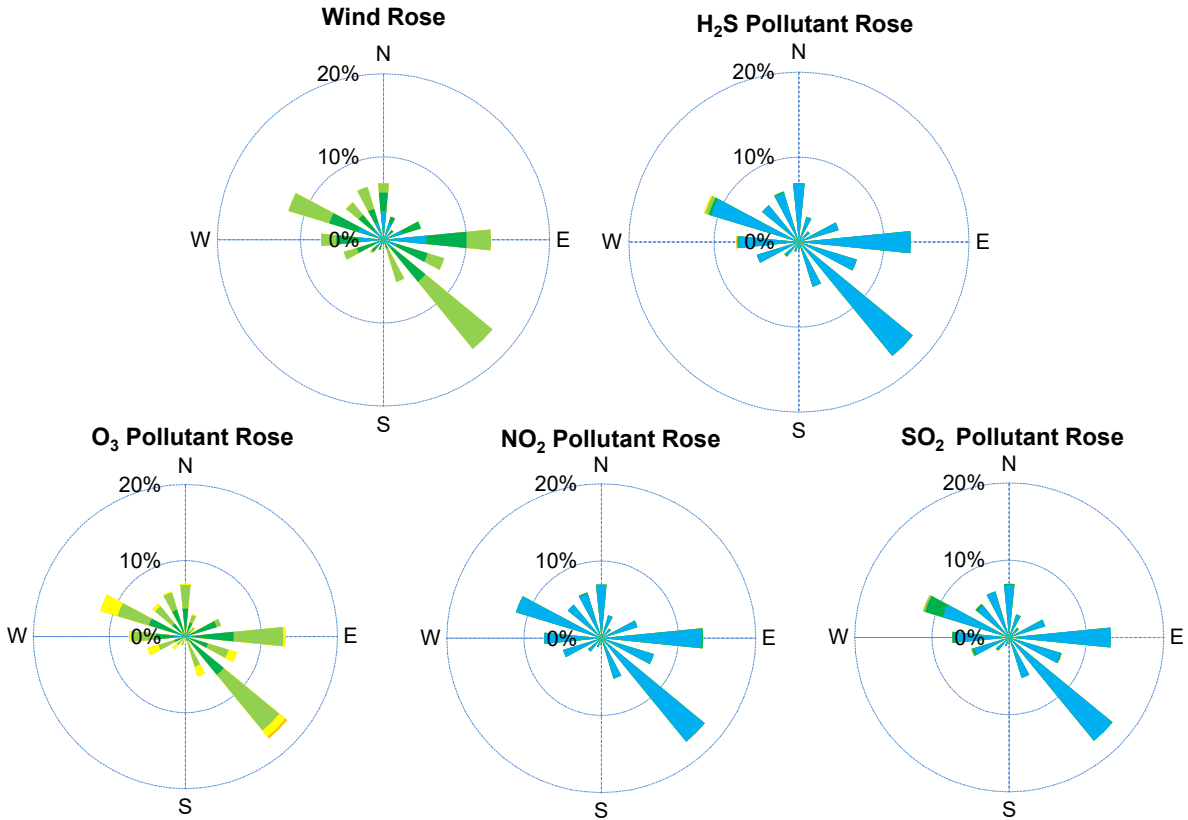

Parameters	Unit	Color Code for Wind Spd & Pollutant Conc. Class						
Wind Speed	m/s	0.3 ≤ WS < 1.4	1.4 ≤ WS < 3.1	3.1 ≤ WS < 7.8	7.8 ≤ WS < 10.8	10.8 ≤ WS < 13.6	WS ≥ 13.6	
SO ₂	ppb	0 ≤ C < 1	1 ≤ C < 5	5 ≤ C < 10	10 ≤ C < 57	57 ≤ C < 172	C ≥ 172	
NO ₂	ppb	0 ≤ C < 5	5 ≤ C < 15	15 ≤ C < 30	30 ≤ C < 100	100 ≤ C < 212	C ≥ 212	
O ₃	ppb	0 ≤ C < 10	10 ≤ C < 20	20 ≤ C < 40	40 ≤ C < 60	60 ≤ C < 82	C ≥ 82	
H ₂ S	ppb	0 ≤ C < 1	1 ≤ C < 3.6	3.6 ≤ C < 5	5 ≤ C < 8	8 ≤ C < 10.8	C ≥ 10.8	




Monthly Update

- *All data has been slope, intercept, and baseline corrected. Data may change after validation process.
- *All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
- *All compliance parameters were more than 90% operational.
- *1 hour of data for NO/NO2/NOX is flagged as "Analyzer Failure" on September 14 due to analyzer issues.
- *Routine quarterly calibrations were completed on September 14 and 18, 2023


SESAA Oxbow Station - September 2023 Summary Report

Pollutants		Month Records		24-Hour Records				1-Hour Records			
Name	Conc. Unit	Avg. Conc.	Uptime	Maximum		SAAQS Standard	Exceed Days	Maximum		SAAQS Standard	Exceed Hours
				Conc.	Time			Conc.	Time		
NO	ppb	#VALUE!	0.0%	< 0.1	#N/A	-	-	< 0.1	-	-	-
NO ₂	ppb	#VALUE!	0.0%	< 0.1	#N/A	106	0	< 0.1	-	159	0
NO _x	ppb	#VALUE!	0.0%	< 0.1	#N/A	-	-	< 0.1	-	-	-
SO ₂	ppb	0.4	100.0%	1.1	Sep-1	48	0	11.2	Sep-18 11:00	172	0
H ₂ S	ppb	0.2	100.0%	0.6	Sep-25	3.6	0	1.9	Sep-21 03:00	11	0
PM _{2.5}	ug/m3	25	66.4%	88	Sep-15	28	6	181	Sep-15 12:00	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards

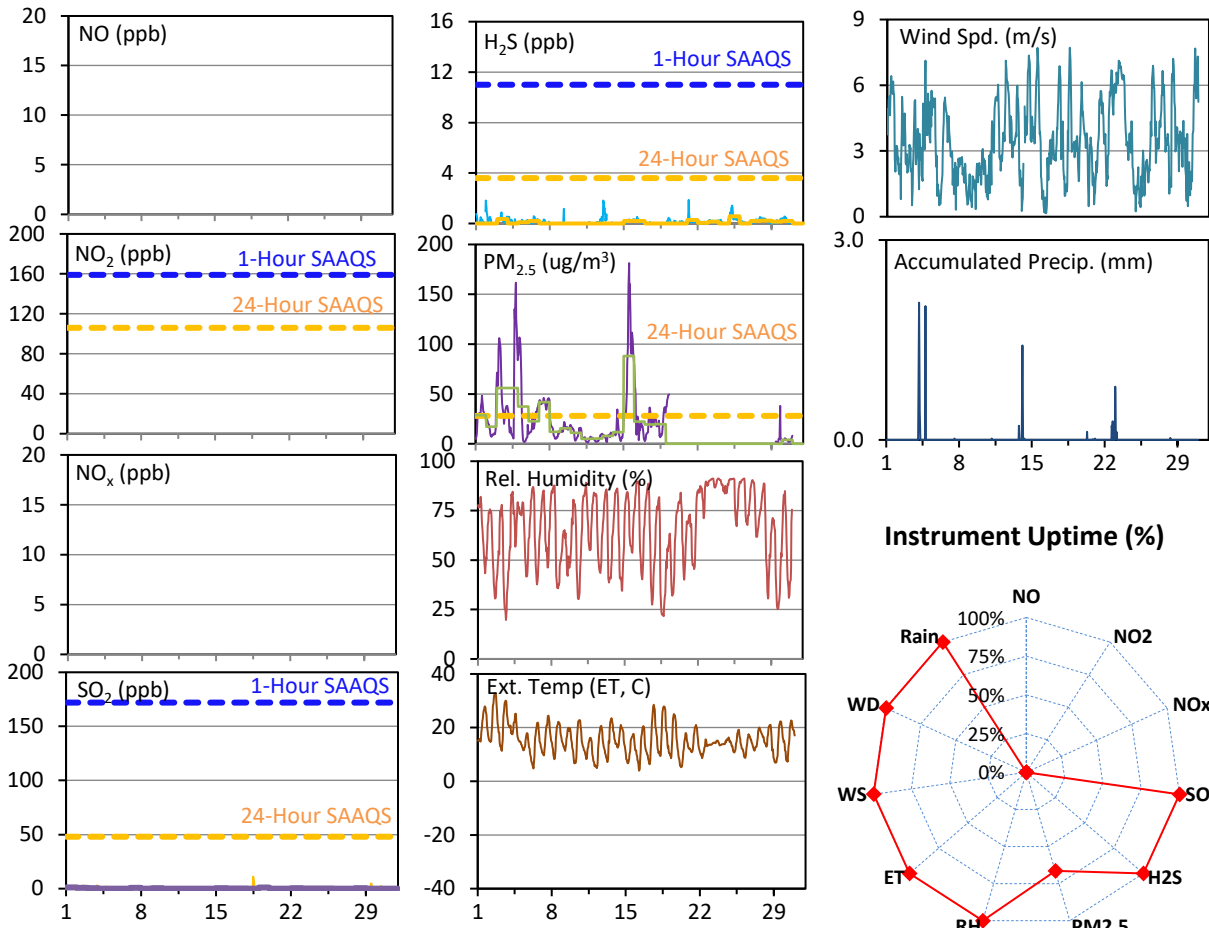

SESAA Oxbow Station - September 2023 Summary Report

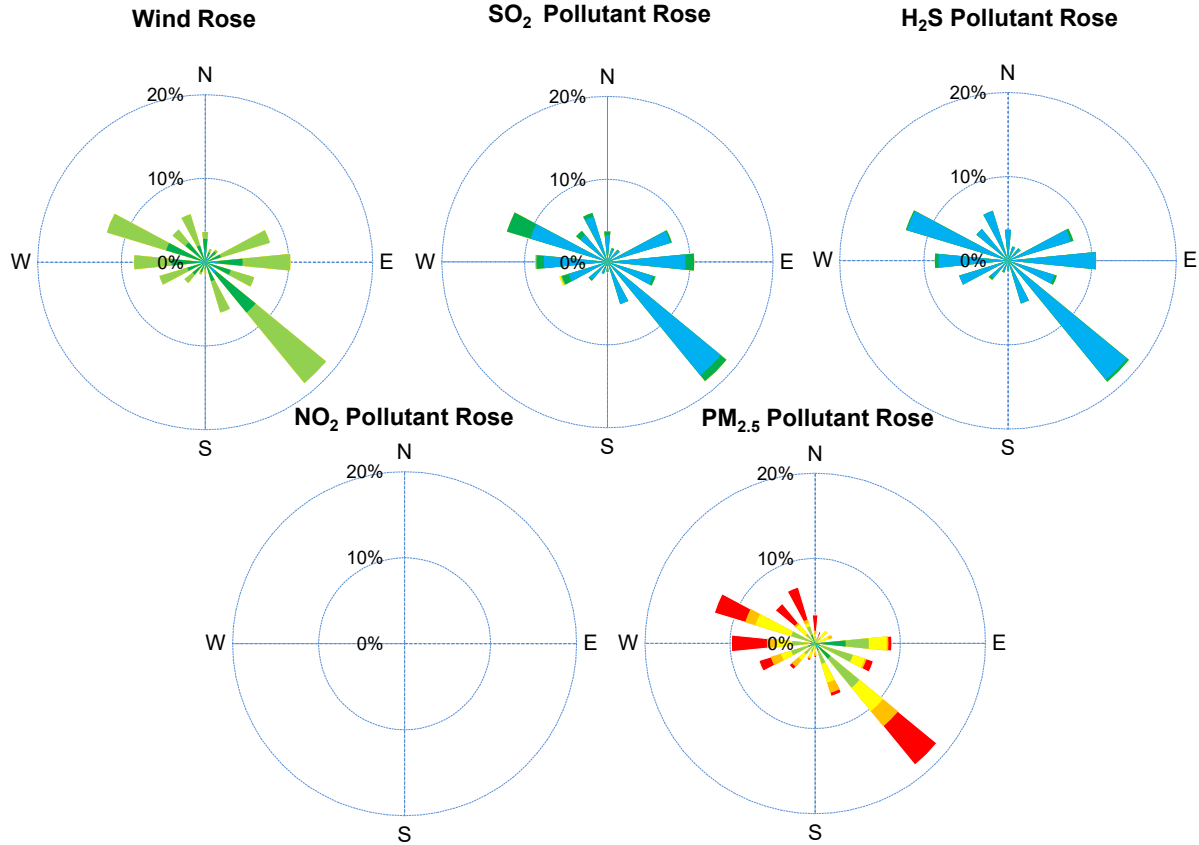

Parameters	Unit	Color Code for Wind Spd & Pollutant Conc. Class					
Wind Speed	m/s	0.3 ≤ WS < 1.4	1.4 ≤ WS < 3.1	3.1 ≤ WS < 7.8	7.8 ≤ WS < 10.8	10.8 ≤ WS < 13.6	WS ≥ 13.6
SO ₂	ppb	0 ≤ C < 1	1 ≤ C < 5	5 ≤ C < 10	10 ≤ C < 57	57 ≤ C < 172	C ≥ 172
NO ₂	ppb	0 ≤ C < 5	5 ≤ C < 15	15 ≤ C < 30	30 ≤ C < 100	100 ≤ C < 212	C ≥ 212
H ₂ S	ppb	0 ≤ C < 1	1 ≤ C < 3.6	3.6 ≤ C < 5	5 ≤ C < 8	8 ≤ C < 10.8	C ≥ 10.8
PM _{2.5}	ug/m ³	0 ≤ C < 2	2 ≤ C < 4	4 ≤ C < 10	10 ≤ C < 20	20 ≤ C < 30	C ≥ 30

Monthly Update

- *All data has been slope, intercept, and baseline corrected. Data may change after validation process.
- *All compliance parameters were within the Saskatchewan Ambient Air Quality Standards with the exception of six 24-hour PM_{2.5} exceedance attributed to wildfire smoke in the area.
- *All compliance parameters were greater than 90% operational, except NO/NO₂/NO_x and PM_{2.5}.
- *242 hours of data flagged as "analyzer failure" for PM_{2.5} due to analyzer malfunction.
- *720 hours of data flagged as "maintenance" for NO/NO₂/NO_x due to analyzer malfunction which needed to be shipped out for maintenance.




Exceedance Summary

24-hour Exceedance Information			Summary of Other Parameters During Exceedance								
Pollutant	24-hr Avg Conc.	Exceedance Date mmm-dd	WS m/s	WD deg	AQI -	Rain mm	ET C	SO ₂ ppb	NO ₂ ppb	H ₂ S ppb	PM _{2.5} ug/m ³
PM _{2.5}	29	Sep-1	4.6	254	-	0.0	20.8	1.1	-	-	29
PM _{2.5}	56	Sep-3	3.0	194	-	0.0	21.0	0.6	-	0.3	56
PM _{2.5}	56	Sep-4	3.7	259	-	0.3	19.3	-	-	-	56
PM _{2.5}	37	Sep-5	3.7	240	-	0.0	13.9	-	-	0.1	37
PM _{2.5}	42	Sep-7	2.2	193	-	0.0	16.6	0.7	-	-	42
PM _{2.5}	88	Sep-15	4.2	296	-	0.0	12.2	0.4	-	0.2	88


SESAA Stoughton Station - September 2023 Summary Report

Pollutants		Month Records		24-Hour Records				1-Hour Records			
Name	Conc. Unit	Avg. Conc.	Uptime	Maximum		SAAQS Standard	Exceed Days	Maximum		SAAQS Standard	Exceed Hours
				Conc.	Time			Conc.	Time		
NO	ppb	< 0.1	1.9%	< 0.1	#N/A	-	-	0.1	Sep-01 00:00	-	-
NO ₂	ppb	0.4	1.9%	< 0.1	#N/A	106	0	3.3	Sep-01 09:00	159	0
NO _x	ppb	0.4	1.9%	< 0.1	#N/A	-	-	3.3	Sep-01 09:00	-	-
SO ₂	ppb	0.3	99.7%	1.1	Sep-3	48	0	4.2	Sep-03 19:00	172	0
H ₂ S	ppb	0.2	99.7%	0.6	Sep-3	3.6	0	2.2	Sep-08 03:00	11	0
PM _{2.5}	ug/m3	20	99.7%	68	Sep-4	28	7	171	Sep-04 17:00	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards

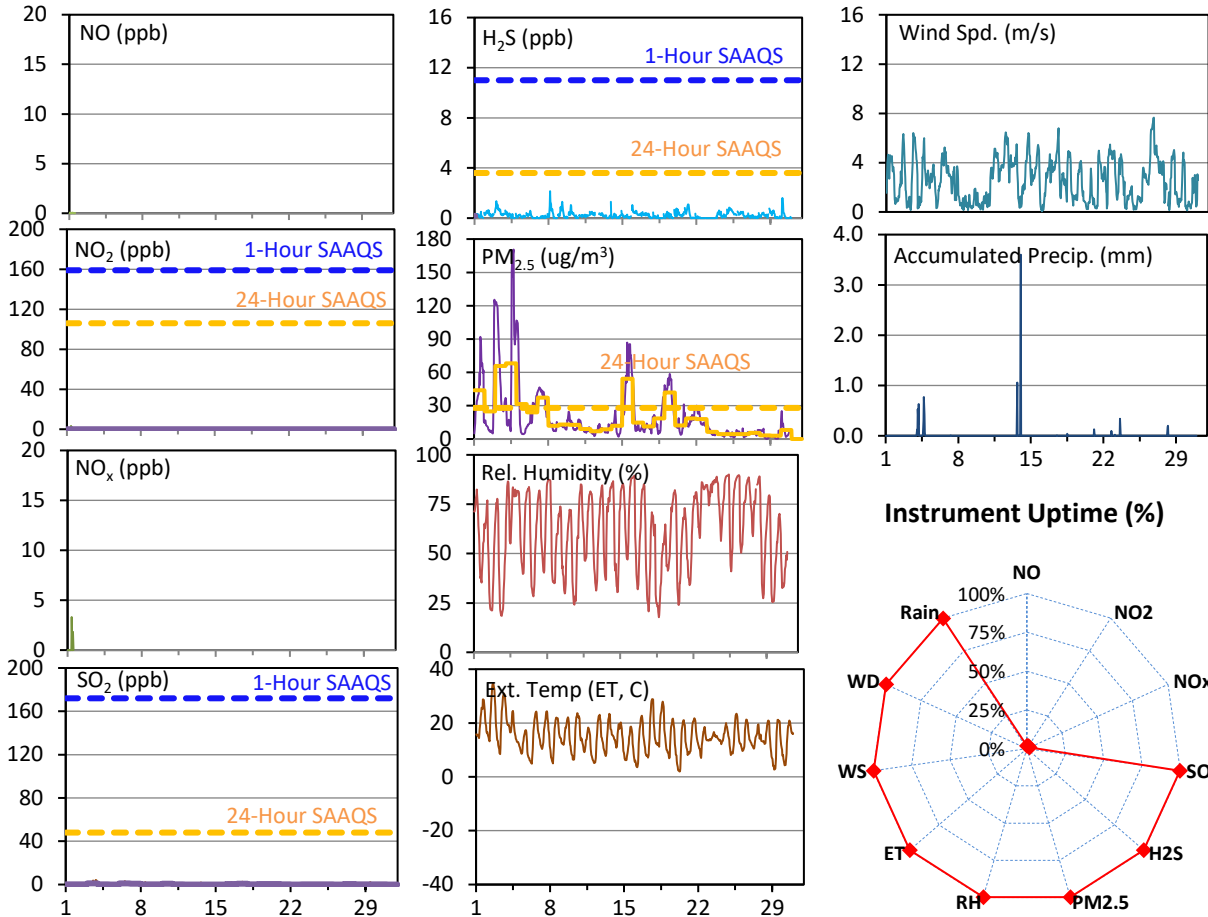

SESAA Stoughton Station - September 2023 Summary Report

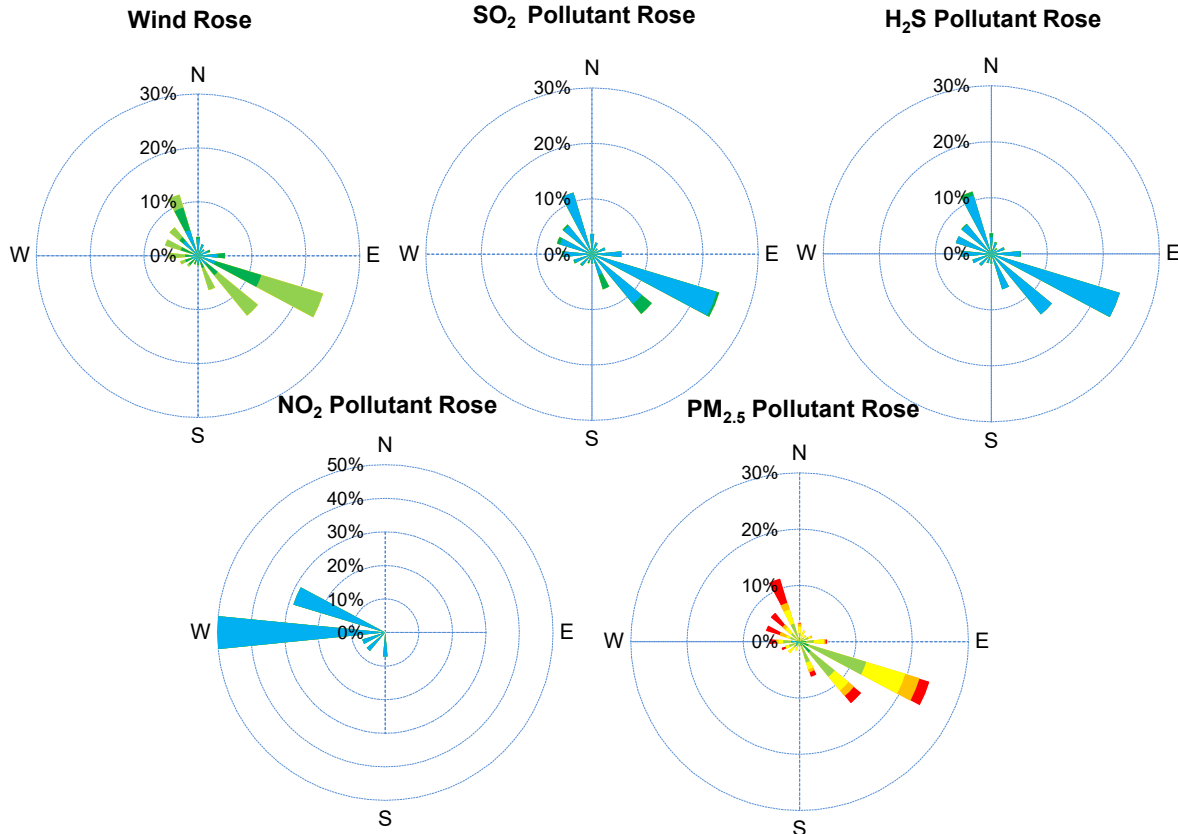

Parameters	Unit	Color Code for Wind Spd & Pollutant Conc. Class						
Wind Speed	m/s	0.3 ≤ WS < 1.4	1.4 ≤ WS < 3.1	3.1 ≤ WS < 7.8	7.8 ≤ WS < 10.8	10.8 ≤ WS < 13.6	WS ≥ 13.6	
SO ₂	ppb	0 ≤ C < 1	1 ≤ C < 5	5 ≤ C < 10	10 ≤ C < 57	57 ≤ C < 172	C ≥ 172	
NO ₂	ppb	0 ≤ C < 5	5 ≤ C < 15	15 ≤ C < 30	30 ≤ C < 100	100 ≤ C < 212	C ≥ 212	
H ₂ S	ppb	0 ≤ C < 1	1 ≤ C < 3.6	3.6 ≤ C < 5	5 ≤ C < 8	8 ≤ C < 10.8	C ≥ 10.8	
PM _{2.5}	ug/m ³	0 ≤ C < 2	2 ≤ C < 4	4 ≤ C < 10	10 ≤ C < 20	20 ≤ C < 30	C ≥ 30	

Monthly Update

- *All data has been slope, intercept, and baseline corrected. Data may change after validation process.
- *All compliance parameters were within the Saskatchewan Ambient Air Quality Standards with the exception of seven 24-hour PM_{2.5} exceedances associated with wildfire smoke in the area.
- *All compliance parameters were greater than 90% operational, except for NO/NO₂/NO_x due to maintenance issues.
- *2 hours of data flagged as "power failure" due to intermittent power issues that occurred at the station.
- *708 hours of data flagged as "maintenance" for NO/NO₂/NO_x on September 1 - 30 due to maintenance issues. Analyzer has been shipped for maintenance.
- *Routine quarterly calibrations were completed on September 12, 2023 except for NO/NO₂/NO_x.


Exceedance Summary (24-Hour Average)

24-hour Exceedance Information			Summary of Other Parameters During Exceedance								
Pollutant (unit)	24-hr Avg Conc.	Exceedance Date mmm-dd	WS m/s	WD deg	AQI -	Rain mm	ET C	SO ₂ ppb	NO ₂ ppb	H ₂ S ppb	PM _{2.5} ug/m ³
PM _{2.5}	44	Sep-1	3.0	256	-	0.0	20.8	0.2	-	0.2	44
PM _{2.5}	66	Sep-3	3.0	185	-	0.0	20.6	1.1	-	0.6	66
PM _{2.5}	68	Sep-4	2.5	270	-	0.1	17.7	0.2	-	0.2	68
PM _{2.5}	31	Sep-5	2.2	307	-	0.0	12.0	-	-	0.2	31
PM _{2.5}	37	Sep-7	2.4	199	-	0.0	16.5	0.7	-	-	37
PM _{2.5}	54.0	Sep-15	2.9	303	-	0.0	11	-	-	0.2	54
PM _{2.5}	42.0	Sep-19	2.2	313	-	0.0	13	0.4	-	0.2	42

SESAA Torquay Station - September 2023 Summary Report

Pollutants		Month Records		24-Hour Records				1-Hour Records			
Name	Conc. Unit	Avg. Conc.	Uptime	Maximum		SAAQS Standard	Exceed Days	Maximum		SAAQS Standard	Exceed Hours
				Conc.	Time			Conc.	Time		
SO ₂	ppb	0.2	100.0%	< 0.1	#N/A	48	0	20.4	Sep-20 17:00	172	0
H ₂ S	ppb	0.3	99.4%	0.7	Sep-4	3.6	0	2.4	Sep-01 20:00	11	0
PM _{2.5}	ug/m3	20	100.0%	74	Sep-4	28	8	204	Sep-04 14:00	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards

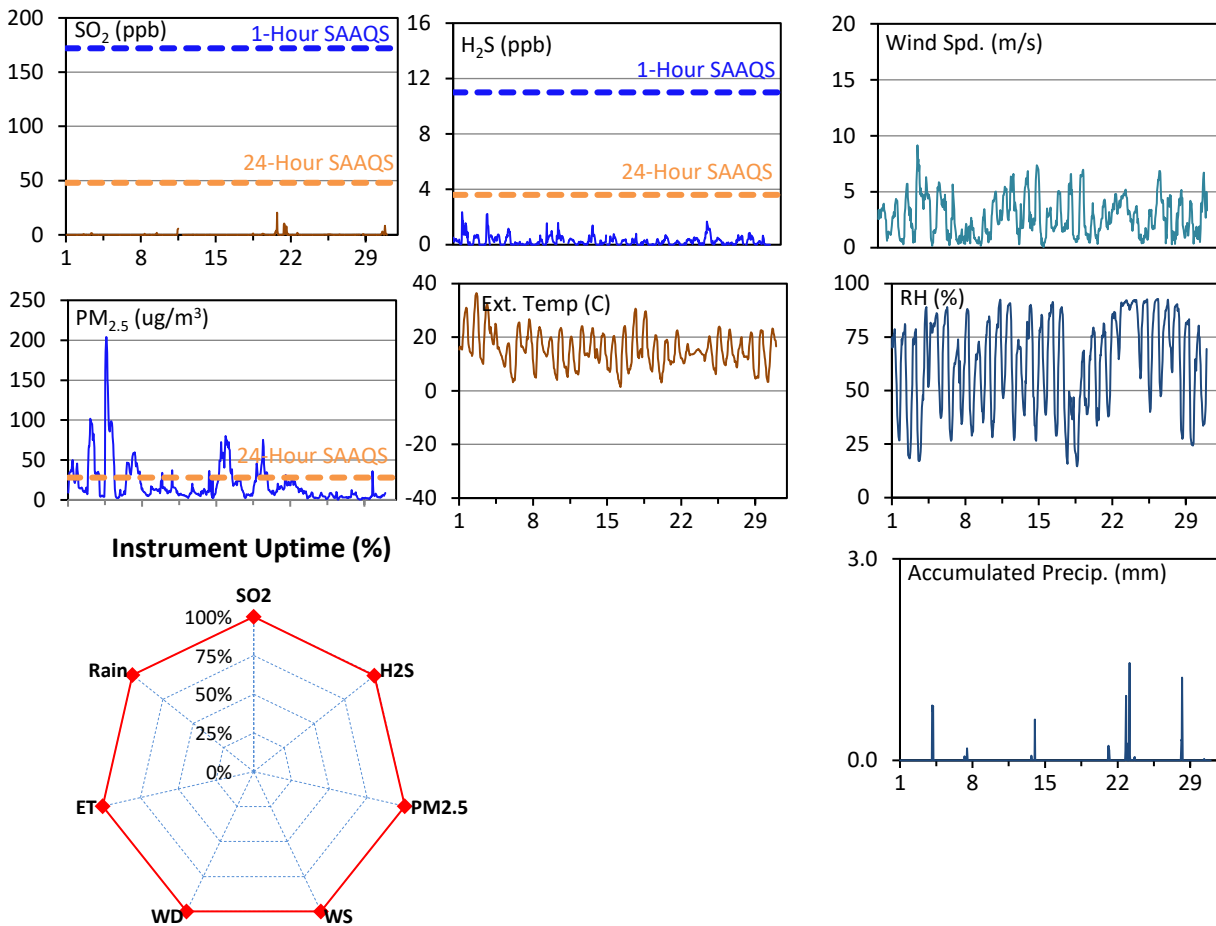


Monthly Update

*All data has been slope, intercept, and baseline corrected. Data may change after validation process.

*All compliance parameters were within the Saskatchewan Ambient Air Quality Standards with the exception of eight 24-hour PM_{2.5} exceedance attributed to wildfire smoke in the area.

*All compliance parameters had greater than 90% operational uptime.

SESAA Torquay Station - September 2023 Summary Report

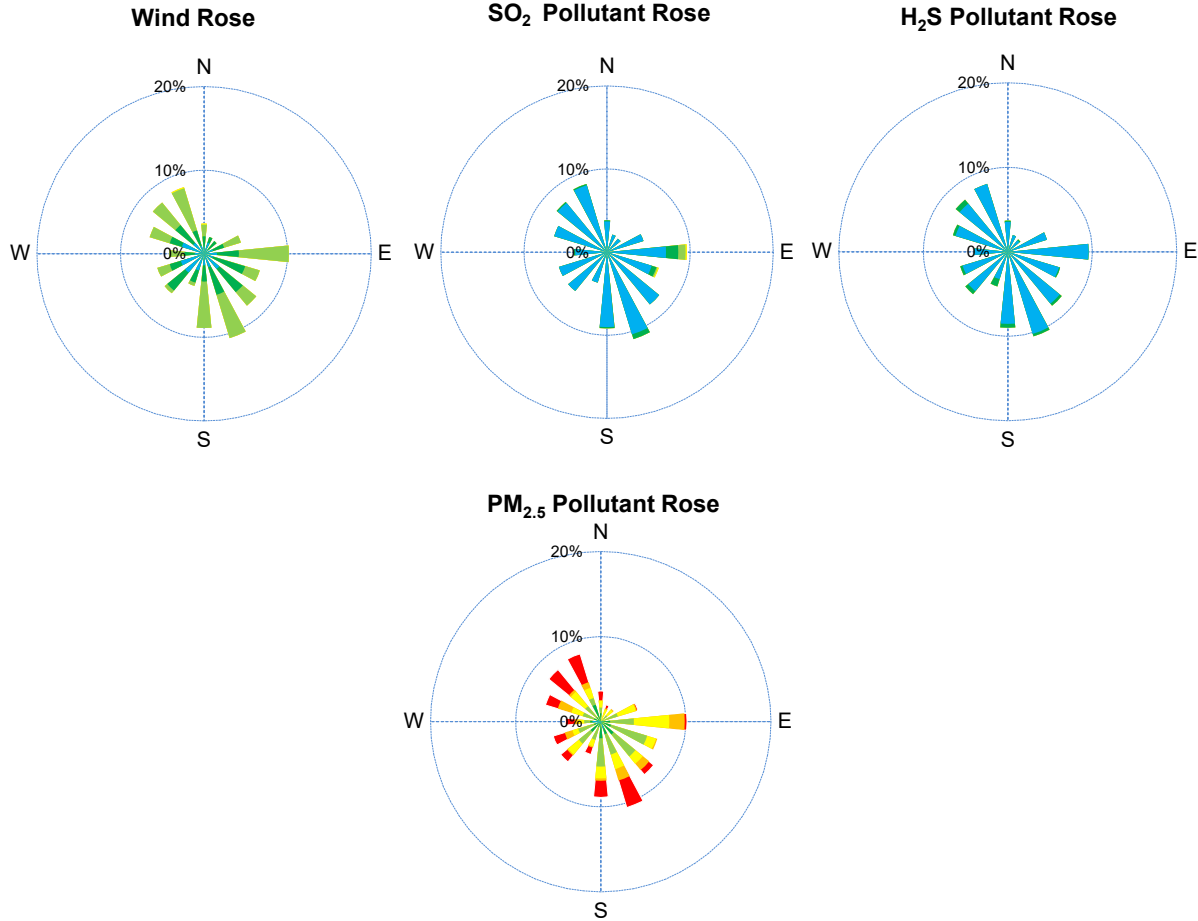




Parameters	Unit	Color Code for Wind Spd & Pollutant Conc. Class					
Wind Speed	m/s	0.3 ≤ WS < 1.4	1.4 ≤ WS < 3.1	3.1 ≤ WS < 7.8	7.8 ≤ WS < 10.8	10.8 ≤ WS < 13.6	WS ≥ 13.6
SO ₂	ppb	0 ≤ C < 1	1 ≤ C < 5	5 ≤ C < 10	10 ≤ C < 57	57 ≤ C < 172	C ≥ 172
NO ₂	ppb	0 ≤ C < 5	5 ≤ C < 15	15 ≤ C < 30	30 ≤ C < 100	100 ≤ C < 212	C ≥ 212
O ₃	ppb	0 ≤ C < 10	10 ≤ C < 20	20 ≤ C < 40	40 ≤ C < 60	60 ≤ C < 82	C ≥ 82
H ₂ S	ppb	0 ≤ C < 1	1 ≤ C < 3.6	3.6 ≤ C < 5	5 ≤ C < 8	8 ≤ C < 10.8	C ≥ 10.8
PM _{2.5}	ug/m ³	0 ≤ C < 2	2 ≤ C < 4	4 ≤ C < 10	10 ≤ C < 20	20 ≤ C < 30	C ≥ 30

Exceedance Summary (24-Hour Average)									
24-hour Exceedance Information			Summary of Other Parameters During Exceedance						
Pollutant	Conc. ppb	Exceedance Date mmm-dd	WS m/s	WD deg	AQHI -	Rain mm	SO2 ppb	H2S ppb	PM2.5 ug/m3
PM2.5	32	Sep-1	2.64	258.81	-	0	-	0.4886	31.71
PM2.5	59	Sep-3	2.64	207.56	-	0	-	-	58.60
PM2.5	74	Sep-4	4.04	289.17	-	0.0983	-	0.6527	74.16
PM2.5	35	Sep-5	3.76	324.61	-	0	-	-	34.52
PM2.5	41	Sep-7	2.49	212.97	-	0.0104	-	-	40.95
PM2.5	48	Sep-15	3.61	282.95	-	0	-	-	48.30
PM2.5	38	Sep-16	1.86	153.4	-	0	-	-	38.15
PM2.5	36	Sep-19	3.29	299.93	-	0	-	-	36.43

SESAA Wauchope Station - September 2023 Summary Report

Pollutants		Month Records		24-Hour Records				1-Hour Records			
Name	Conc. Unit	Avg. Conc.	Uptime	Maximum		SAAQS Objective	Exceed Days	Maximum		SAAQS Objective	Exceed Hours
				Conc.	Time			Conc.	Time		
SO ₂	ppb	0.2	100.0%	0.9	Sep-2	48	0	3.3	Sep-02 12:00	172	0
H ₂ S	ppb	0.6	99.9%	0.9	Sep-30	3.6	0	14.6	Sep-10 03:00	11	5
PM _{2.5}	ug/m ³	18	100.0%	65	Sep-3	28	6	153	Sep-04 18:00	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards

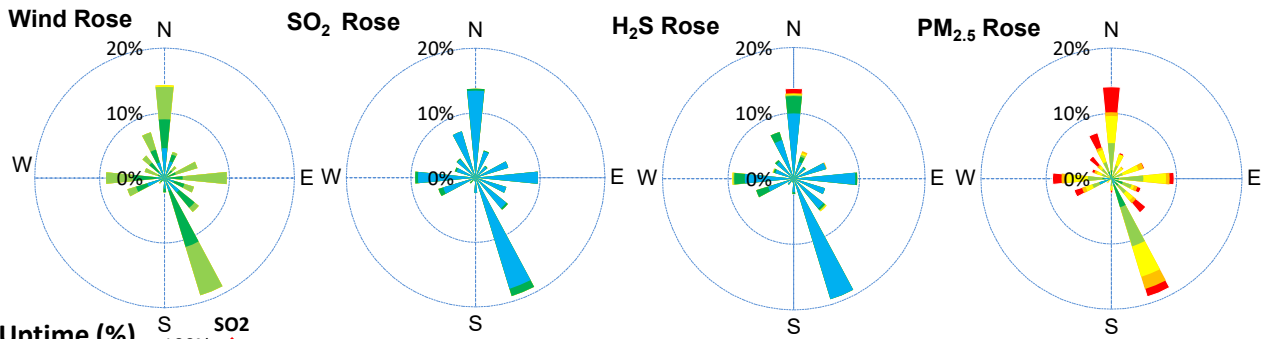

Parameters	Unit	Color Code for Wind Spd & Pollutant Conc. Class					
Wind Speed	m/s	0.3 ≤ WS < 1.4	1.4 ≤ WS < 3.1	3.1 ≤ WS < 7.8	7.8 ≤ WS < 10.8	10.8 ≤ WS < 13.6	WS ≥ 13.6
SO ₂	ppb	0 ≤ C < 1	1 ≤ C < 5	5 ≤ C < 10	10 ≤ C < 57	57 ≤ C < 172	C ≥ 172
H ₂ S	ppb	0 ≤ C < 1	1 ≤ C < 3.6	3.6 ≤ C < 5	5 ≤ C < 8	8 ≤ C < 10.8	C ≥ 10.8
PM _{2.5}	ug/m ³	0 ≤ C < 2	2 ≤ C < 4	4 ≤ C < 10	10 ≤ C < 20	20 ≤ C < 30	C ≥ 30

SESAA Wauchope Station - September 2023 Summary Report

Exceedance Summary (1-Hour Average)

1-hour Exceedance Information			Summary of Other Parameters During Exceedance						
Pollutant	Conc. ppb	Exceedance Time mmm-dd hh:mm	WS m/s	WD deg	Rain mm	ET C	SO ₂ ppb	H ₂ S ppb	PM _{2.5} ug/m3
H2S	14.0	Sep-06 00:00	0.4	4	0.0	4.9	0.0	14.0	12
H2S	11.1	Sep-06 05:00	0.0	4	0.0	4.7	0.0	11.1	28
H2S	11.4	Sep-10 02:00	0.4	355	0.0	6.4	0.0	11.4	9
H2S	14.6	Sep-10 03:00	0.3	7	0.0	6.2	0.0	14.6	9
H2S	13.0	Sep-10 05:00	0.6	359	0.0	5.0	0.0	13.0	7

Exceedance Summary (24-Hour Average)

24-hour Exceedance Information			Summary of Other Parameters During Exceedance						
Pollutant	Conc. ppb	Exceedance Date mmm-dd	WS m/s	WD deg	Rain mm	ET C	SO ₂ ppb	H ₂ S ppb	PM _{2.5} ug/m3
PM2.5	65	Sep-3	1.7	192	0.0	21.5	0.3	-	65
PM2.5	64.0	Sep-4	4.0	176	0.4	18.7	0.2	0.8	64
PM2.5	38.0	Sep-5	3.9	278	0.0	12.4	-	-	38
PM2.5	39.0	Sep-7	1.9	198	0.1	15	0.3	0.4	39
PM2.5	38.0	Sep-15	3.6	282	0.0	12	-	-	38
PM2.5	32.0	Sep-19	2.6	285	0.0	16	-	-	32


Monthly Update

- *All data has been slope, intercept, and baseline corrected. Data may change after validation process.
- *All compliance parameters were within the Saskatchewan Ambient Air Quality Standards with the exception of six 24-hour PM 2.5 exceedances associated with wildfire smoke in the area. Five 1-hour H2S exceedances were also recorded.
- *All compliance parameters were greater than 90% operational.
- *1 hour of data for H2S is flagged as "analyzer failure" due to an analyzer issue on site.
- *Routine quarterly calibrations were completed on September 19, 2023.


SESAA Weyburn Station - September 2023 Summary Report

Pollutants		Month Records		24-Hour Records				1-Hour Records			
Name	Conc. Unit	Avg. Conc.	Uptime	Maximum		SAAQS Standard	Exceed Days	Maximum		SAAQS Standard	Exceed Hours
				Conc.	Time			Conc.	Time		
NO	ppb	-	0.0%	< 0.1	#N/A	-	-	< 0.1	-	-	-
NO ₂	ppb	-	0.0%	< 0.1	#N/A	106	0	< 0.1	-	159	0
NO _x	ppb	-	0.0%	< 0.1	#N/A	-	-	< 0.1	-	-	-
SO ₂	ppb	0.6	1.5%	< 0.1	#N/A	48	0	3.2	Sep-01 00:00	172	0
O ₃	ppb	26	1.5%	< 1	#N/A	-	-	30	Sep-01 10:00	82	0
H ₂ S	ppb	0.3	1.5%	< 0.1	#N/A	3.6	0	0.5	Sep-01 07:00	11	0
PM _{2.5}	ug/m3	41	1.5%	< 1	#N/A	28	0	74	Sep-01 10:00	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards

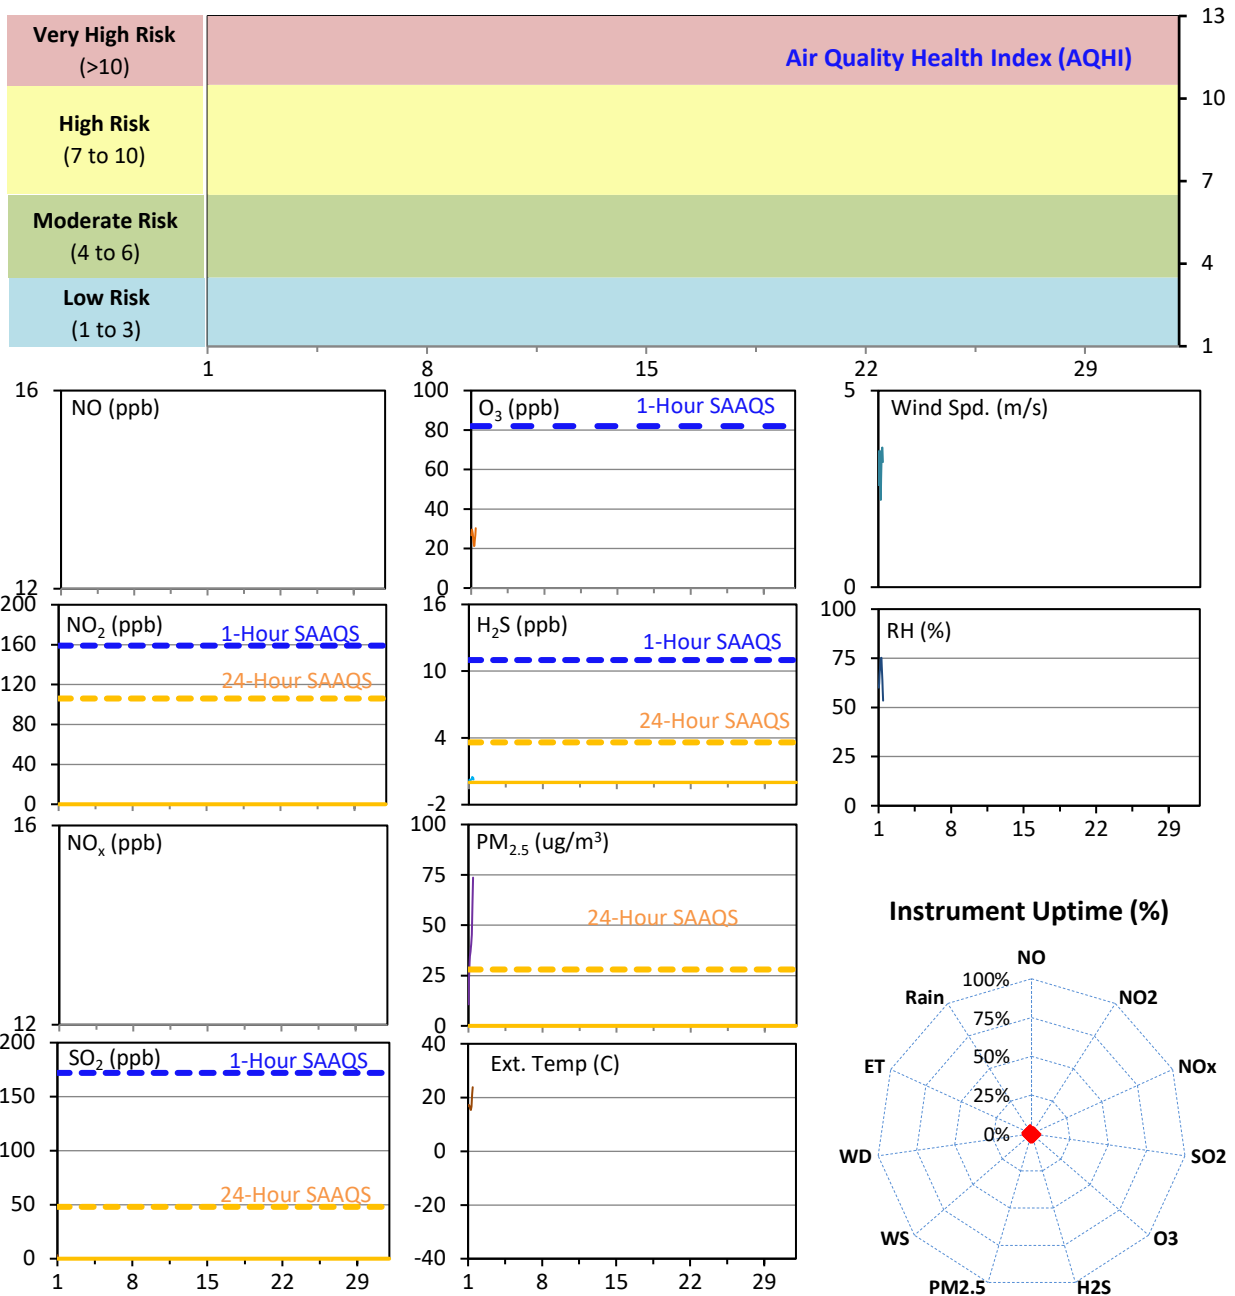

SESAA Weyburn Station - September 2023 Summary Report

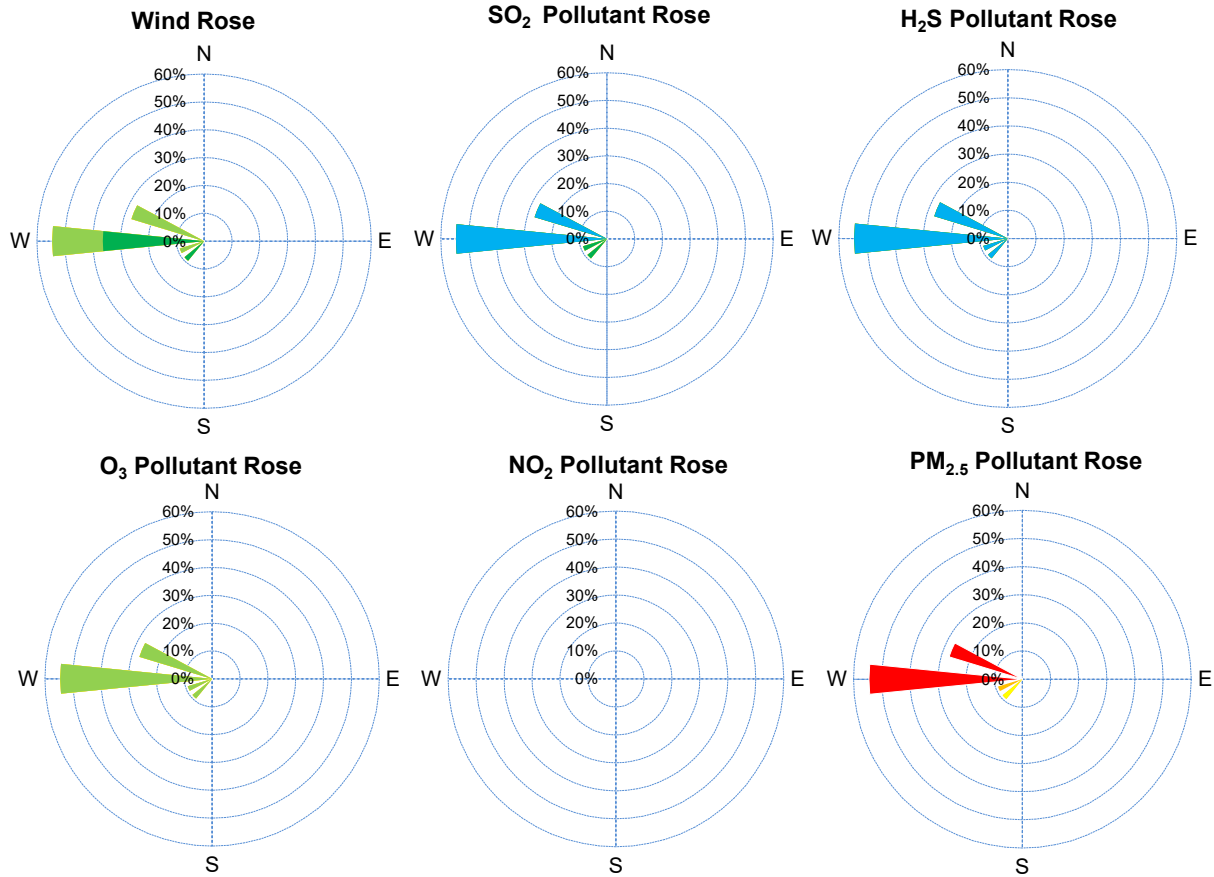

Parameters	Unit	Color Code for Wind Spd & Pollutant Conc. Class						
Wind Speed	m/s	$0.3 \leq WS < 1.4$	$1.4 \leq WS < 3.1$	$3.1 \leq WS < 7.8$	$7.8 \leq WS < 10.8$	$10.8 \leq WS < 13.6$	$WS \geq 13.6$	
SO ₂	ppb	$0 \leq C < 1$	$1 \leq C < 5$	$5 \leq C < 10$	$10 \leq C < 57$	$57 \leq C < 172$	$C \geq 172$	
NO ₂	ppb	$0 \leq C < 5$	$5 \leq C < 15$	$15 \leq C < 30$	$30 \leq C < 100$	$100 \leq C < 212$	$C \geq 212$	
O ₃	ppb	$0 \leq C < 10$	$10 \leq C < 20$	$20 \leq C < 40$	$40 \leq C < 60$	$60 \leq C < 82$	$C \geq 82$	
H ₂ S	ppb	$0 \leq C < 1$	$1 \leq C < 3.6$	$3.6 \leq C < 5$	$5 \leq C < 8$	$8 \leq C < 10.8$	$C \geq 10.8$	
PM _{2.5}	ug/m ³	$0 \leq C < 2$	$2 \leq C < 4$	$4 \leq C < 10$	$10 \leq C < 20$	$20 \leq C < 30$	$C \geq 30$	

Monthly Update

- *All data has been slope, intercept, and baseline corrected. Data may change after validation process.
- *All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
- *All compliance parameters were less than 90% operational due to maintenance issues with the whole station.
- *720 hours of data for NO/NO2/NOx are flagged as "maintenance" as the analyzer was removed from service on June 3.
- *709 hours of data for all parameters except NO/NO2/NOx are flagged as "maintenance" as the station was been taken out of service on September 1.
- *Parts have been ordered for station repair.
- *Routine quarterly calibrations were not completed due to maintenance issues.