










## SESAA Esterhazy Station - October 2024 Summary Report

Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS Objective	Exceed Days	Maximum		SAAQS Objective	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
NO	ppb	0.5	95.2%	1.5	7-Oct	-	-	18.2	10/7/2024 08:00	-	-
NO <sub>2</sub>	ppb	1.5	95.2%	3.7	31-Oct	106	0	12.3	10/31/2024 06:00	159	0
NO <sub>x</sub>	ppb	2	95.2%	4.1	31-Oct	-	-	29.4	10/7/2024 08:00	-	-
O <sub>3</sub>	ppb	8.5	94.9%	29.6	19-Oct	-	-	42.5	10/4/2024 17:00	82	0
PM <sub>2.5</sub>	µg/m <sup>3</sup>	6.3	98.8%	11.1	10-Oct	28	0	38.3	10/28/2024 23:00	-	-


SAAQS: Saskatchewan Ambient Air Quality Standards

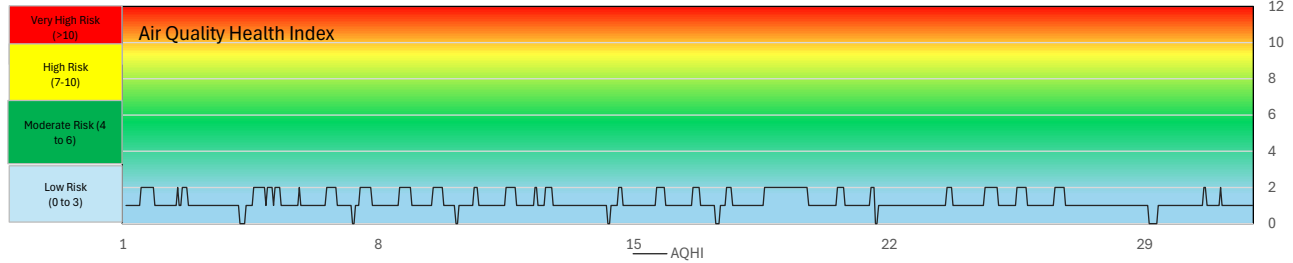


### Exceedance Summary

24-hour Exceedance Information			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	Precip.	NO	NO <sub>2</sub>	NO <sub>x</sub>	O <sub>3</sub>	PM <sub>2.5</sub>


# SESAA Esterhazy Station - October 2024 Summary Report




Wind Rose



Pollution Rose NO<sub>2</sub>



Pollution Rose O<sub>3</sub>



Pollution Rose PM<sub>2.5</sub>

Parameters	Unit	Color Code for Wind Speed and Pollutant Conc. Class						
Wind Speed	m/s	0.5 -W- 1.2	1.2 -W- 2.4	2.4 -W- 3.6	3.6 -W- 4.8	4.8 -W- 6.0	W > 6.0	
NO <sub>2</sub>	ppb	0.0-C-3.0	3.0-C-6.0	6.0-C-9.0	9.0-C-12.0	12.0-C-15.0	C > 15.0	
O <sub>3</sub>	ppb	0.0-C-8.0	8.0-C-16.0	16.0-C-24.0	24.0-C-32.0	32.0-C-40.0	C > 40.0	
PM <sub>2.5</sub>	µg/m <sup>3</sup>	0.0-C-8.0	8.0-C-16.0	16.0-C-24.0	24.0-C-32.0	32.0-C-40.0	C > 40.0	










\* All data has been zero baseline corrected, if any. Data may change after final validation process.  
 \* All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.  
 \* All compliance parameters were less than 90% operational for the month.  
 \* NO/NO<sub>2</sub>/NO<sub>x</sub>, O<sub>3</sub> and PM<sub>2.5</sub> analyzer calibrations performed during the week of October 21, 2024.



# SESAA Glen Ewen Station - October 2024 Summary Report


Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQs Objective	Exceed Days	Maximum		SAAQs Objective	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
NO	ppb	0.4	85.8%	0.99	27-Oct	-	-	7.3	10/27/2024 08:00	-	-
NO <sub>2</sub>	ppb	1.4	85.8%	3.63	29-Oct	106	0	10.1	10/29/2024 08:00	159	0
NO <sub>x</sub>	ppb	1.8	85.8%	4.61	29-Oct	-	-	14.3	10/31/2024 07:00	-	-
SO <sub>2</sub>	ppb	0.3	85.6%	0.95	9-Oct	48	0	6.2	10/9/2024 11:00	172	0
H <sub>2</sub> S	ppb	1.5	85.6%	1.83	20-Oct	3.6	0	2.9	10/24/2024 03:00	11	0
O <sub>3</sub>	µg/m <sup>3</sup>	23.7	85.8%	34.19	5-Oct	-	-	52.4	10/8/2024 16:00	82	0

SAAQs: Saskatchewan Ambient Air Quality Standards

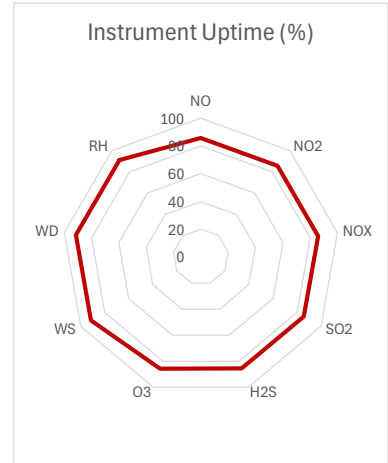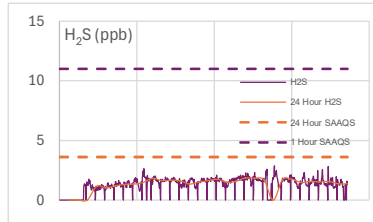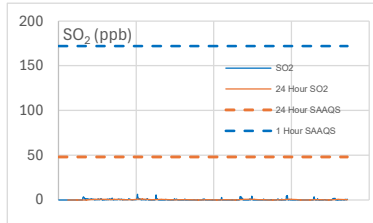


# SESAA Glen Ewen Station - October 2024 Summary Report


Exceedance Summary										
24-hour Exceedance Information			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	H <sub>2</sub> S	NO	NO <sub>2</sub>	NO <sub>x</sub>	SO <sub>2</sub>	O <sub>3</sub>




Wind Rose




NO<sub>2</sub> Pollution Rose



SO<sub>2</sub> Pollution Rose



H<sub>2</sub>S Pollution Rose



O<sub>3</sub> Pollution Rose

Parameters	Unit	Color Code for Wind Speed and Pollutant Conc. Class						
Wind Speed	m/s	0.5 -W- 1.2	1.2 -W- 2.4	2.4 -W- 3.6	3.6 -W- 4.8	4.8 -W- 6.0	W > 6.0	
NO <sub>2</sub>	ppb	0.0-C-2.0	2.0-C-4.0	4.0-C-6.0	6.0-C-8.0	8.0-C-10.0	C > 10.0	
SO <sub>2</sub>	ppb	0.0-C-0.8	0.8-C-1.6	1.6-C-2.4	2.4-C-3.2	3.2-C-4.0	C > 4.0	
H <sub>2</sub> S	ppb	0.0-C-1.0	1.0-C-2.0	2.0-C-3.0	3.0-C-4.0	4.0-C-5.0	C > 5.0	
O <sub>3</sub>	µg/m3	0.0-C-10.0	10.0-C-20.0	20.0-C-30.0	30.0-C-40.0	40.0-C-50.0	C > 50.0	

## Monthly Update










- \* All data has been baseline corrected. Data may change after final validation process.
- \* All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
- \* All compliance parameters were less than 90% operational for the month, due to extended power failure.
- \* NO/NO<sub>2</sub>/NO<sub>x</sub>, O<sub>3</sub>, SO<sub>2</sub> and H<sub>2</sub>S analyzers calibrated the weeks of October 21 and 28, 2024.



# SESAA Oxbow Station - October 2024 Summary Report


Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS Objective	Exceed Days	Maximum		SAAQS Objective	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
NO	ppb	0.5	93.8%	0.7	23-Oct	-	-	2.3	10/23/2024 10:00	-	-
NO <sub>2</sub>	ppb	1.6	93.8%	2.5	29-Oct	106	0	5.4	10/24/2024 08:00	159	0
NO <sub>x</sub>	ppb	2.1	93.8%	2.9	29-Oct	-	-	6.1	10/24/2024 08:00	-	-
SO <sub>2</sub>	ppb	0.7	93.8%	1.4	30-Oct	48	0	5.2	10/30/2024 12:00	172	0
H <sub>2</sub> S	ppb	0.1	94.0%	0.2	7-Oct	3.6	0	1.9	10/29/2024 02:00	11	0
PM <sub>2.5</sub>	µg/m <sup>3</sup>	7.7	27.0%	13.3	8-Oct	28	0	34.5	10/8/2024 21:00	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards




# SESAA Oxbow Station - October 2024 Summary Report


Exceedance Summary										
24-hour Exceedance Information			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	H <sub>2</sub> S	NO	NO <sub>2</sub>	NO <sub>x</sub>	SO <sub>2</sub>	PM <sub>2.5</sub>




Wind Rose




NO<sub>2</sub> Pollution Rose



SO<sub>2</sub> Pollution Rose



H<sub>2</sub>S Pollution Rose



PM<sub>2.5</sub> Pollution Rose










Monthly Update
<ul style="list-style-type: none"> <li>* All data has been zero baseline corrected. Data may change after final validation process.</li> <li>* All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.</li> <li>* All compliance parameters were more than 90% operational for the month, except for PM<sub>2.5</sub> and WS/WD.</li> <li>* 720 hours of data flagged as " analyzer failure" for WS/WD due to missing data. Sensor not reporting data as of August 6, 2024. Sensor removed on October 31, 2024 for maintenance.</li> <li>* 543 hours of data flagged as "analyzer failure" for PM<sub>2.5</sub> due to missing and flatlined data.</li> <li>* 30 hours of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.</li> <li>* NO/NO<sub>2</sub>/NO<sub>x</sub>, O<sub>3</sub>, SO<sub>2</sub>, H<sub>2</sub>S and PM<sub>2.5</sub> analyzers were calibrated the weeks of October 7 and 28, 2024.</li> </ul>



# SESAA Stoughton Station - October 2024 Summary Report


Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS Objective	Exceed Days	Maximum		SAAQS Objective	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
NO	ppb	0.4	94.8%	0.8	24-Oct	-	-	11.8	14/10/2024 15:00	-	-
NO <sub>2</sub>	ppb	1.3	94.8%	2.6	31-Oct	106	0	7.9	04/10/2024 05:00	159	0
NO <sub>x</sub>	ppb	1.7	94.8%	3.1	31-Oct	-	-	12.0	14/10/2024 15:00	-	-
SO <sub>2</sub>	ppb	0.9	94.6%	1.9	27-Oct	48	0	5.7	04/10/2024 22:00	172	0
H <sub>2</sub> S	ppb	0.7	94.6%	1.8	27-Oct	3.6	0	4.0	11/10/2024 07:00	11	0
PM <sub>2.5</sub>	µg/m <sup>3</sup>	7.1	99.9%	15.0	8-Oct	28	0	27.9	16/10/2024 21:00	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards




# SESAA Stoughton Station - October 2024 Summary Report


Exceedance Summary										
24-hour Exceedance Information			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	H <sub>2</sub> S	NO	NO <sub>2</sub>	NO <sub>x</sub>	SO <sub>2</sub>	PM <sub>2.5</sub>




Wind Rose




NO<sub>2</sub> Pollution Rose



SO<sub>2</sub> Pollution Rose



H<sub>2</sub>S Pollution Rose



PM<sub>2.5</sub> Pollution Rose

Parameters	Unit	Color Code for Wind Speed and Pollutant Conc. Class						
Wind Speed	m/s	0.5 -W- 1.2	1.2 -W- 2.4	2.4 -W- 3.6	3.6 -W- 4.8	4.8 -W- 6.0	W > 6.0	
NO <sub>2</sub>	ppb	0.0-C-1.6	1.6-C-3.2	3.2-C-4.8	4.8-C-6.4	6.4-C-8.0	C > 8.0	
SO <sub>2</sub>	ppb	0.0-C-1.2	1.2-C-2.4	2.4-C-3.6	3.6-C-C4.8	4.8-C-6.0	C > 6.0	
H <sub>2</sub> S	ppb	0.0-C-1.0	1.0-C-2.0	2.0-C-3.0	3.0-C-4.0	4.0-C-5.0	C > 5.0	
PM <sub>2.5</sub>	µg/m <sup>3</sup>							

## Monthly Update

- \* All data has been zero baseline corrected, if any. Data may change after final validation process.
- \* All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
- \* All compliance parameters were more than 90% operational for the month except for PM<sub>2.5</sub>.
- \* The PM<sub>2.5</sub> raw beta data has been manually downloaded from the Airpointer website. It represents unvalidated beta data and is intended for reference purposes only. Mass concentration data is unavailable as the instrument is malfunctioning. Consequently, the pollution rose analysis has not been generated.
- \* 30 hours of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
- \* NO<sub>x</sub>, SO<sub>2</sub>, H<sub>2</sub>S and PM<sub>2.5</sub> analyzers were calibrated on the week of October 7, 2024.











## SESAA Torquay Station - October 2024 Summary Report


SESAA Torquay Station - October 2024 Summary Report											
Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS Objective	Exceed Days	Maximum		SAAQS Objective	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
SO <sub>2</sub>	ppb	0.8	93.8%	1.2	9-Oct	48	0	5.2	10/14/2024 12:00	172	0
H <sub>2</sub> S	ppb	0.3	94.2%	1.4	8-Oct	3.6	0	2.7	10/8/2024 22:00	11	0
PM <sub>2.5</sub>	µg/m <sup>3</sup>	6.1	99.1%	16.0	16-Oct	28	0	46.8	10/16/2024 19:00	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards




Exceedance Summary								
24-hour Exceedance Information			Summary of other Parameters during Exceedance					
Pollutant	Date	Conc.	WS	WD	Precip.	SO <sub>2</sub>	H <sub>2</sub> S	PM <sub>2.5</sub>


# SESAA Torquay Station - October 2024 Summary Report




Wind Rose



Pollution Rose SO<sub>2</sub>



Pollution Rose H<sub>2</sub>S



Pollution Rose PM<sub>2.5</sub>

Parameters	Unit	Color Code for Wind Speed and Pollutant Conc. Class						
Wind Speed	m/s	0.5 -W- 1.2	1.2 -W- 2.4	2.4 -W- 3.6	3.6 -W- 4.8	4.8 -W- 6.0	W > 6.0	
SO <sub>2</sub>	ppb	0.0-C-1.0	1.0-C-2.0	2.0-C-3.0	3.0-C-4.0	4.0-C-5.0	C > 5.0	
H <sub>2</sub> S	ppb	0.0-C-1.0	1.0-C-2.0	2.0-C-3.0	3.0-C-4.0	4.0-C-5.0	C > 5.0	
PM <sub>2.5</sub>	µg/m3	0.0-C-8.0	8.0-C-16.0	16.0-C-24.0	24.0-C-32.0	32.0-C-40.0	C > 40.0	

## Monthly Update







- \* All data has been zero baseline corrected, if any. Data may change after final validation process.
- \* All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
- \* All compliance parameters were more than 90% operational for the month.
- \* 30 hours of data were flagged due to daily IZS checks, resulting in the loss of one hour of data each day.
- \* SO<sub>2</sub>, H<sub>2</sub>S and PM<sub>2.5</sub> analyzers were calibrated the weeks of October 7 and 28, 2024.



## SESAA Wauchope Station - October 2024 Summary Report

Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS Objective	Exceed Days	Maximum		SAAQS Objective	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
SO <sub>2</sub>	ppb	1	94.8%	1.7	1-Oct	48	0	6	16/10/2024 14:00	172	0
H <sub>2</sub> S	ppb	0.6	94.8%	2.1	10-Oct	3.6	0	16.18	10/10/2024 03:00	11	1
PM <sub>2.5</sub>	µg/m <sup>3</sup>	7.1	99.5%	15.5	9-Oct	28	0	31.1	21/10/2024 19:00	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards




### Exceedance Summary (24-Hour Average)


24-hour Exceedance Information			Summary of other Parameters during Exceedance					
Pollutant	Date	Conc.	WS	WD	Precip.	SO <sub>2</sub>	H <sub>2</sub> S	PM <sub>2.5</sub>

# SESAA Wauchope Station - October 2024 Summary Report


Exceedance Summary (1-Hour Average)									
1-hour Exceedance Information				Summary of Other Parameters During Exceedance					
Pollutant	Date	Time	Conc.	WS	WD	Precip.	SO <sub>2</sub>	H <sub>2</sub> S	PM <sub>2.5</sub>
H <sub>2</sub> S	10-Oct	3:00 AM	16.2	0.2	70.4	0.0	1.2	16.2	16.7




Wind Rose



Pollution Rose SO<sub>2</sub>



Pollution Rose H<sub>2</sub>S



Pollution Rose PM<sub>2.5</sub>

Parameters	Unit	Color Code for Wind Speed and Pollutant Conc. Class						
Wind Speed	m/s	0.5 -W- 1.2	1.2 -W- 2.4	2.4 -W- 3.6	3.6 -W- 4.8	4.8 -W- 6.0	W > 6.0	
SO <sub>2</sub>	ppb	0.0-C-1.0	1.0-C-2.0	2.0-C-3.0	3.0-C-4.0	4.0-C-5.0	C > 5.0	
H <sub>2</sub> S	ppb	0.0-C-2.0	2.0-C-4.0	4.0-C-6.0	6.0-C-8.0	8.0-C-10.0	C > 10.0	
PM <sub>2.5</sub>	µg/m <sup>3</sup>	0.0-C-5.0	5.0-C-10.0	10.0-C-15.0	15.0-C-20.0	20.0-C-25.0	C > 25.0	

## Monthly Update










- \* All data has been zero baseline corrected, if any. Data may change after final validation process.
- \* All compliance parameters were within the Saskatchewan Ambient Air Quality Standards with the exception of one 24 hour H<sub>2</sub>S exceedance.
- \* All compliance parameters were more than 90% operational for the month.
- \* 30 hours of data were flagged due to daily IZS checks, resulting in the loss of one hour of data each day.
- \* SO<sub>2</sub>, H<sub>2</sub>S and PM<sub>2.5</sub> analyzers were calibrated the weeks of October 21 and 28, 2024.



# SESAA Weyburn Station - October 2024 Summary Report

Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS Objective	Exceed Days	Maximum		SAAQS Objective	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
NO	ppb	0.2	95.0%	0.8	2-Oct	-	-	4.4	30/10/2024 08:00	-	-
NO <sub>2</sub>	ppb	1.9	95.0%	2.8	27-Oct	106	0	6.9	09/10/2024 18:00	159	0
NO <sub>x</sub>	ppb	1.6	95.0%	2.5	8-Oct	-	-	7.2	09/10/2024 18:00	-	-
SO <sub>2</sub>	ppb	1.0	20.6%	1.8	1-Oct	48	0	12.0	01/10/2024 24:00	172	0
H <sub>2</sub> S	ppb	0.7	20.6%	0.9	2-Oct	3.6	0	5.5	02/10/2024 03:00	11	0
PM <sub>2.5</sub>	µg/m <sup>3</sup>	5.8	99.5%	12.0	8-Oct	28	0	44.0	08/10/2024 18:00	-	-



SAAQS: Saskatchewan Ambient Air Quality Standards



# SESAA Weyburn Station - October 2024 Summary Report

Exceedance Summary (24-Hours Average)										
24-hours Exceedance Information			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	H <sub>2</sub> S	NO	NO <sub>2</sub>	NOx	SO <sub>2</sub>	PM <sub>2.5</sub>

Exceedance Summary (1-Hour Average)										
1-hour Exceedance Information				Summary of Other Parameters During Exceedance						
Pollutant	Date	Time	Conc.	WS	WD	Precip.	SO <sub>2</sub>	NO <sub>2</sub>	PM <sub>2.5</sub>	



Parameters	Unit	Color Code for Wind Speed and Pollutant Conc. Class						
Wind Speed	m/s	0.5 -W- 1.2	1.2 -W- 2.4	2.4 -W- 3.6	3.6 -W- 4.8	4.8 -W- 6.0	W > 6.0	
NO <sub>2</sub>	ppb	0.0-C-1.2	1.2-C-2.4	2.4-C-3.6	3.6-C-4.8	4.8-C-6.0	C > 6.0	
SO <sub>2</sub>	ppb	0.0-C-0.8	0.8-C-1.6	1.6-C-2.4	2.4-C-3.2	3.2-C-4.0	C > 4.0	
H <sub>2</sub> S	ppb	0.0-C-0.6	0.6-C-1.2	1.2-C-1.8	1.8-C-2.4	2.4-C-3.0	C > 3.0	
PM <sub>2.5</sub>	µg/m <sup>3</sup>	0.0-C-8.0	8.0-C-16.0	16.0-C-24.0	24.0-C-32.0	32.0-C-40.0	C > 40.0	

**Monthly Update**

- \* All data has been zero baseline corrected, if any. Data may change after final validation process.
- \* All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
- \* All compliance parameters were more than 90% operational for the month except for H<sub>2</sub>S and SO<sub>2</sub>.
- \* 591 hours of data flagged as "analyzer failure" for H<sub>2</sub>S and SO<sub>2</sub> due to missing and flatlined data.
- \* 30 hours of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
- \* NOx and PM<sub>2.5</sub> analyzers were calibrated the week of October 7, 2024. Further evaluation of H<sub>2</sub>S and SO<sub>2</sub> analyzer required.

