






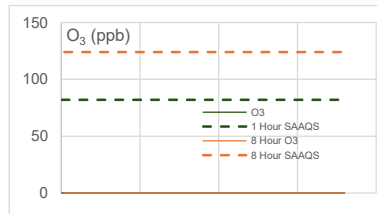


SESAA Esterhazy Station - November 2025 Summary Report


Pollutant		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Concentration	Date and Time		
NO	ppb	No Data	0.0%	0.0	-	-	-	No Data	-	-	-
NO ₂	ppb	No Data	0.0%	0.0	-	106	0	No Data	-	159	-
NO _x	ppb	No Data	0.0%	0.0	-	-	-	No Data	-	-	-
O ₃	ppb	No Data	0.0%	0.0	-	124 (8-Hour)	0	No Data	-	82	0
PM _{2.5}	µg/m ³	No Data	0.0%	0.0	-	28	0	No Data	-	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards




Exceedance Summary										
24-hour Exceedance Information			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	Precip.	NO	NO ₂	NO _x	O ₃	PM _{2.5}


SESAA Esterhazy Station - November 2025 Summary Report

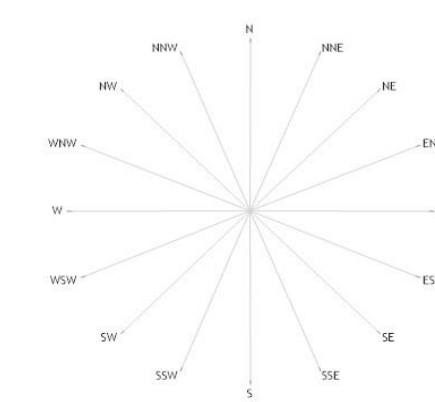


Wind Rose



Pollution Rose NO₂

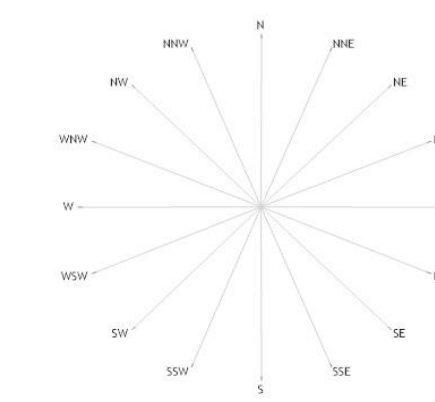

Pollution Rose O₃



Pollution Rose PM_{2.5}

Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class					
Wind Speed	m/s	N/A	N/A	N/A	N/A	N/A	N/A
NO ₂	ppb	N/A	N/A	N/A	N/A	N/A	N/A
O ₃	ppb	N/A	N/A	N/A	N/A	N/A	N/A
PM _{2.5}	µg/m ³	N/A	N/A	N/A	N/A	N/A	N/A










* System was shut down on July 5, 2025 due to HVAC system malfunctioned.
 * Most recent quarterly calibrations were completed on April 26, 2025.



SESAA Glen Ewen Station - November 2025 Summary Report

Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
NO	ppb	0.2	94.7%	0.7	11/16/2025	-	-	6.1	11/21/2025 8:00 AM	-	-
NO ₂	ppb	1.5	94.7%	2.7	11/16/2025	106	0	7.5	11/5/2025 7:00 PM	159	0
NO _x	ppb	1.6	94.7%	3.4	11/16/2025	-	-	12.9	11/21/2025 8:00 AM	-	-
SO ₂	ppb	1	94.7%	1.4	11/22/2025	48	0	3.4	11/6/2025 4:00 PM	172	0
H ₂ S	ppb	0.5	94.7%	1.4	11/4/2025	3.6	0	21.2	11/4/2025 8:00 PM	11	1
O ₃	ppb	21.3	94.7%	36.2	11/3/2025	124 (8 hours)	0	40.4	11/4/2025 2:00 PM	82	0

SAAQS: Saskatchewan Ambient Air Quality Standards





SESAA Glen Ewen Station - November 2025 Summary Report

Exceedance Summary (24-Hour Average)

24-hour Exceedance Information			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	H ₂ S	NO	NO ₂	NO _x	SO ₂	O ₃

Exceedance Summary (1-Hour Average)

1-hour Exceedance Information				Summary of Other Parameters During Exceedance					
Pollutant	Date and Time	Conc.	WS	WD	Precip.	SO ₂	NO ₂	O ₃	
H ₂ S	4-Nov 8:00:00 PM	21.2	2.05	272.5	0.0	1.0	1.7	25.5	

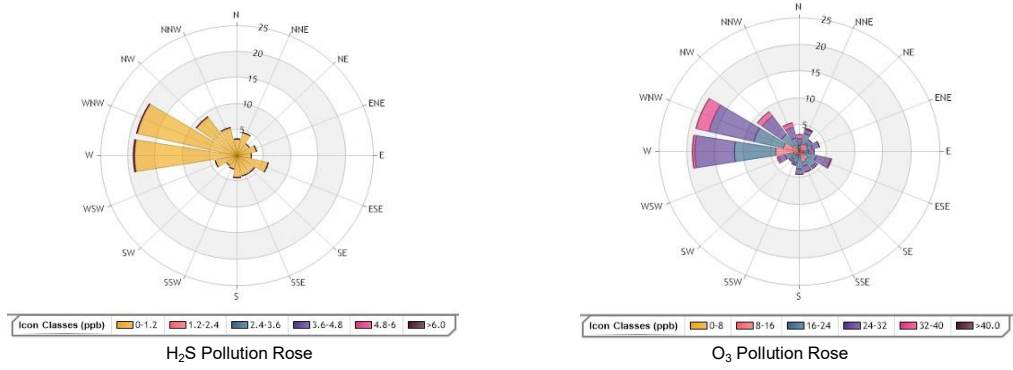

Parameters	Unit	Color Code for Wind Speed and Pollutant Conc. Class						
Wind Speed	m/s	0.5 -W- 1.2	1.2 -W- 2.4	2.4 -W- 3.6	3.6 -W- 4.8	4.8 -W- 6.0	W > 6.0	
NO ₂	ppb	0.0 -C- 1.2	1.2 -C- 2.4	2.4 -C- 3.6	3.6 -C- 4.8	4.8 -C- 6.0	C > 6.0	
SO ₂	ppb	0.0 -C- 1.2	1.2 -C- 2.4	2.4 -C- 3.6	3.6 -C- 4.8	4.8 -C- 6.0	C > 6.0	
H ₂ S	ppb	0.0 -C- 1.2	1.2 -C- 2.4	2.4 -C- 3.6	3.6 -C- 4.8	4.8 -C- 6.0	C > 6.0	
O ₃	ppb	0.0 -C- 8.0	8.0 -C- 16.0	16.0 -C- 24.0	24.0 -C- 32.0	32.0 -C- 40.0	C > 40.0	

Monthly Update


- * All data has been zero drift and baseline corrected, if needed. Data may change after final validation process.
- * All compliance parameters were within the Saskatchewan Ambient Air Quality Standards with the exception of one H₂S one-hour exceedance.
- * All compliance parameters were greater than 90% operational for the month.
- * The NO₂ permeation tube was depleted, and as a result, daily span checks were not included in the data process.
- * One hour of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
- * Quarterly calibrations were completed on November 30, 2025.




SESAA Oxbow Station - November 2025 Summary Report

Exceedance Summary


Exceedance Information			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	H ₂ S	NO	NO ₂	NO _x	SO ₂	PM _{2.5}




Wind Rose




NO₂ Pollution Rose

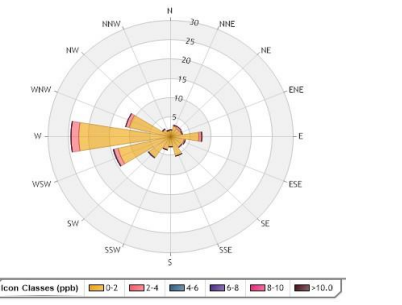

SO₂ Pollution Rose



H₂S Pollution Rose



PM_{2.5} Pollution Rose

Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class						
Wind Speed	m/s	0.5 -W- 1.2	1.2 -W- 2.4	2.4 -W- 3.6	3.6 -W- 4.8	4.8 -W- 6.0	W > 6.0	
NO ₂	ppb	0.0-C- 1.2	1.2 -C- 2.4	2.4-C- 3.6	3.6-C- 4.8	4.8 -C- 6.0	C > 6.0	
SO ₂	ppb	0.0-C-2.0	2.0-C-4.0	4.0-C-6.0	6.0-C-8.0	8.0-C-10.0	C > 10.0	
H ₂ S	ppb	0.0-C-2.0	2.0-C-4.0	4.0-C-6.0	6.0-C-8.0	8.0-C-10.0	C > 10.0	
PM _{2.5}	µg/m ³	0.0-C-3.0	3.0-C-6.0	6.0-C-9.0	9.0-C-12.0	12.0-C-15.0	C > 15.0	

Monthly Update


- * All data has been zero drift and baseline corrected, if needed. Data may change after final validation process.
- * All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
- * All compliance parameters were more than 90% operational for the month, except for PM_{2.5}
- * A total of 667 hours of PM_{2.5} data intermittent throughout the month were flagged as "analyzer malfunction," resulting in missing and flatlined data.
- * The NO₂ permeation tube was depleted, and as a result, daily span checks were not included in the data process.
- * One hour of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
- * Quarterly calibrations were completed on November 28, 2025.




SESAA Stoughton Station - November 2025 Summary Report

Exceedance Summary


Exceedance Summary			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	H ₂ S	NO	NO ₂	NO _x	SO ₂	PM _{2.5}




Wind Rose




NO₂ Pollution Rose



SO₂ Pollution Rose



H₂S Pollution Rose



PM_{2.5} Pollution Rose

Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class					
Wind Speed	m/s	N/A	N/A	N/A	N/A	N/A	N/A
NO ₂	ppb	N/A	N/A	N/A	N/A	N/A	N/A
SO ₂	ppb	N/A	N/A	N/A	N/A	N/A	N/A
H ₂ S	ppb	N/A	N/A	N/A	N/A	N/A	N/A
PM _{2.5}	µg/m ³	N/A	N/A	N/A	N/A	N/A	N/A

Monthly Update







* PM_{2.5} was removed from service in December 2024 for repair. Weather station was removed on July 28, 2025. System was shut down on July 31, 2025.
 * System was restarted on November 15, 2025. Calibrations not completed until December 2026. Values are for reference only and have not been validated
 * Most recent quarterly calibrations were completed on April 22, 2025



SESAA Torquay Station - November 2025 Summary Report


Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
SO ₂	ppb	0.6	93.3%	1.2	11/24/2025	48	0	2.9	11/9/2025 3:00 AM	172	0
H ₂ S	ppb	0.0	10.1%	0.0	11/28/2025	3.6	0	0.0	11/27/2025 9:00 PM	11	0
PM _{2.5}	µg/m ³	4.6	91.8%	10.1	11/20/2025	28	0	31.6	11/28/2025 2:00 AM	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards




Exceedance Summary								
24-hour Exceedance Information			Summary of other Parameters during Exceedance					
Pollutant	Date	Conc.	WS	WD	Precip.	SO ₂	H ₂ S	PM _{2.5}


SESAA Torquay Station - November 2025 Summary Report




Wind Rose



Pollution Rose SO₂



Pollution Rose H₂S



Pollution Rose PM_{2.5}

Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class						
Wind Speed	m/s	0.5 -W- 1.2	1.2 -W- 2.4	2.4 -W- 3.6	3.6 -W- 4.8	4.8 -W- 6.0	W > 6.0	
SO ₂	ppb	0.0-C-0.6	0.6-C-1.2	1.2-C-1.8	1.8-C-2.4	2.4-C-3.0	C > 3.0	
H ₂ S	ppb	0.0-C-0.6	0.6-C-1.2	1.2-C-1.8	1.8-C-2.4	2.4-C-3.0	C > 3.0	
PM _{2.5}	µg/m ³	0.0-C-4.0	4.0-C-8.0	8.0-C-12.0	12.0-C-16.0	16.0-C-20.0	C > 20.0	

Monthly Update







- * All data has been zero drift and baseline corrected, where required. Data may change after final validation process.
- * All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
- * All compliance parameters were more than 90% operational for the month except for H₂S.
- * H₂S monitor reinstalled on November 27, 2025 and no permeation tube available for daily span check.
- * One hour of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
- * Most recent quarterly calibrations were completed on November 27, 2025.



SESAA Wauchope Station - November 2025 Summary Report

Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
SO ₂	ppb	0.2	94.3%	0.7	11/21/2025	48	0	3.5	11/21/2025 3:00 PM	172	0
H ₂ S	ppb	No Data	0.0%	0.0	NA	3.6	0	No Data	NA	11	0
PM _{2.5}	µg/m ³	No Data	0.0%	0.0	NA	28	0	No Data	NA	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards




Exceedance Summary (24-Hour Average)


24-hour Exceedance Information			Summary of other Parameters during Exceedance					
Pollutant	Date	Conc.	WS	WD	Precip.	SO ₂	H ₂ S	PM _{2.5}

SESAA Wauchope Station - November 2025 Summary Report


Exceedance Summary (1-Hour Average)								
1-hour Exceedance Information			Summary of Other Parameters During Exceedance					
Pollutant	Date and Time	Conc.	WS	WD	Precip.	SO ₂	H ₂ S	PM _{2.5}




Wind Rose



Pollution Rose SO₂



Pollution Rose H₂S



Pollution Rose PM_{2.5}

Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class					
Wind Speed	m/s	N/A	N/A	N/A	N/A	N/A	N/A
SO ₂	ppb	N/A	N/A	N/A	N/A	N/A	N/A
H ₂ S	ppb	N/A	N/A	N/A	N/A	N/A	N/A
PM _{2.5}	µg/m ³	N/A	N/A	N/A	N/A	N/A	N/A

Monthly Update










- * All data has been zero baseline corrected, where required. Data may change after final validation process.
- * All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
- * All compliance parameters were less 90% operational for the month except for SO₂.
- * A total of 720 hours of data flagged as "analyzer failure" for WS/WD
- * A total of 720 hours of data flagged as analyzer malfunctioning for H₂S.
- * A total of 720 hours of data flagged as analyzer malfunctioning for PM_{2.5}.
- * One hour of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
- * Most recent quarterly calibrations were completed on July 28, 2025.



SESAA Weyburn Station - November 2025 Summary Report

Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
NO	ppb	0.8	93.1%	1.3	11/19/2025	-	-	4.4	11/24/2025 9:00 AM	-	-
NO ₂	ppb	1.2	93.1%	2.1	11/13/2025	106	0	5.6	11/19/2025 1:00 AM	159	0
NO _x	ppb	2.0	93.1%	3.4	11/19/2025	-	-	7.7	11/19/2025 8:00 AM	-	-
SO ₂	ppb	1.8	93.1%	4.8	11/9/2025	48	0	40.3	11/9/2025 3:00 PM	172	0
H ₂ S	ppb	1.1	93.1%	1.7	11/4/2025	3.6	0	10.1	11/15/2025 8:00 PM	11	0
PM _{2.5}	µg/m ³	5.9	14.4%	10.0	11/27/2025	28	0	24.2	11/26/2025 8:00 PM	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards




SESAA Weyburn Station - November 2025 Summary Report

Exceedance Summary (24-Hours Average)

24-hours Exceedance Information			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	H ₂ S	NO	NO ₂	NO _x	SO ₂	PM _{2.5}

Exceedance Summary (1-Hour Average)


1-hour Exceedance Information			Summary of Other Parameters During Exceedance					
Pollutant	Date and Time	Conc.	WS	WD	Precip.	SO ₂	NO ₂	PM _{2.5}

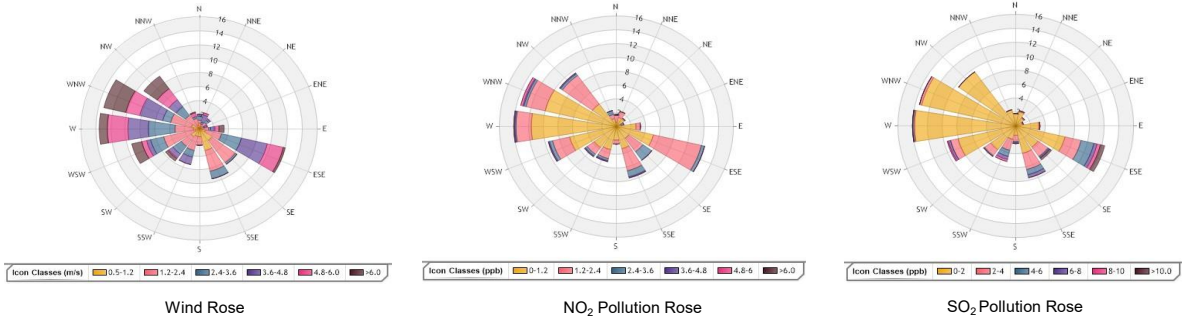

Wind Rose

NO₂ Pollution Rose

SO₂ Pollution Rose



H₂S Pollution Rose

PM_{2.5} Pollution Rose

Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class						
Wind Speed	m/s	0.5-W-1.2	1.2-W-2.4	2.4-W-3.6	3.6-W-4.8	4.8-W-6.0	W > 6.0	
NO ₂	ppb	0.0-C-1.2	1.2-C-2.4	2.4-C-3.6	3.6-C-4.8	4.8-C-6.0	C > 6.0	
SO ₂	ppb	0.0-C-2.0	2.0-C-4.0	4.0-C-6.0	6.0-C-8.0	8.0-C-10.0	C > 10.0	
H ₂ S	ppb	0.0-C-2.0	2.0-C-4.0	4.0-C-6.0	6.0-C-8.0	8.0-C-10.0	C > 10.0	
PM _{2.5}	µg/m ³	0.0-C-4.0	4.0-C-8.0	8.0-C-12.0	12.0-C-16.0	16.0-C-20.0	C > 20.0	

Monthly Update

- * All data has been zero drift and baseline corrected, where required. Data may change after final validation process.
- * All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
- * All compliance parameters were more than 90% operational for the month with the exception of PM_{2.5}.
- * PM_{2.5} monitor was reinstalled on November 26, 2025.
- * One hour of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
- * The SO₂ and NO₂ permeation tube was depleted, and as a result, daily span checks were not included in the data process.
- * Most recent quarterly calibrations were completed on November 26, 2025

