



SESAA Esterhazy Station - March 2026 Summary Report

Pollutant		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Concentration	Date and Time		
NO	ppb	No Data	0.0%	0.0	-	-	-	No Data	0	-	-
NO ₂	ppb	No Data	0.0%	0.0	-	106	0	No Data	0	159	-
NO _x	ppb	No Data	0.0%	0.0	-	-	-	No Data	0	-	-
O ₃	ppb	No Data	0.0%	0.0	-	63 (8-Hour)	0	No Data	0	82	0
PM _{2.5}	µg/m ³	No Data	0.0%	0.0	-	28	0	No Data	0	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards




*If AQHI cannot be calculated due to missing parameters, AQHI plus is reported using PM_{2.5}

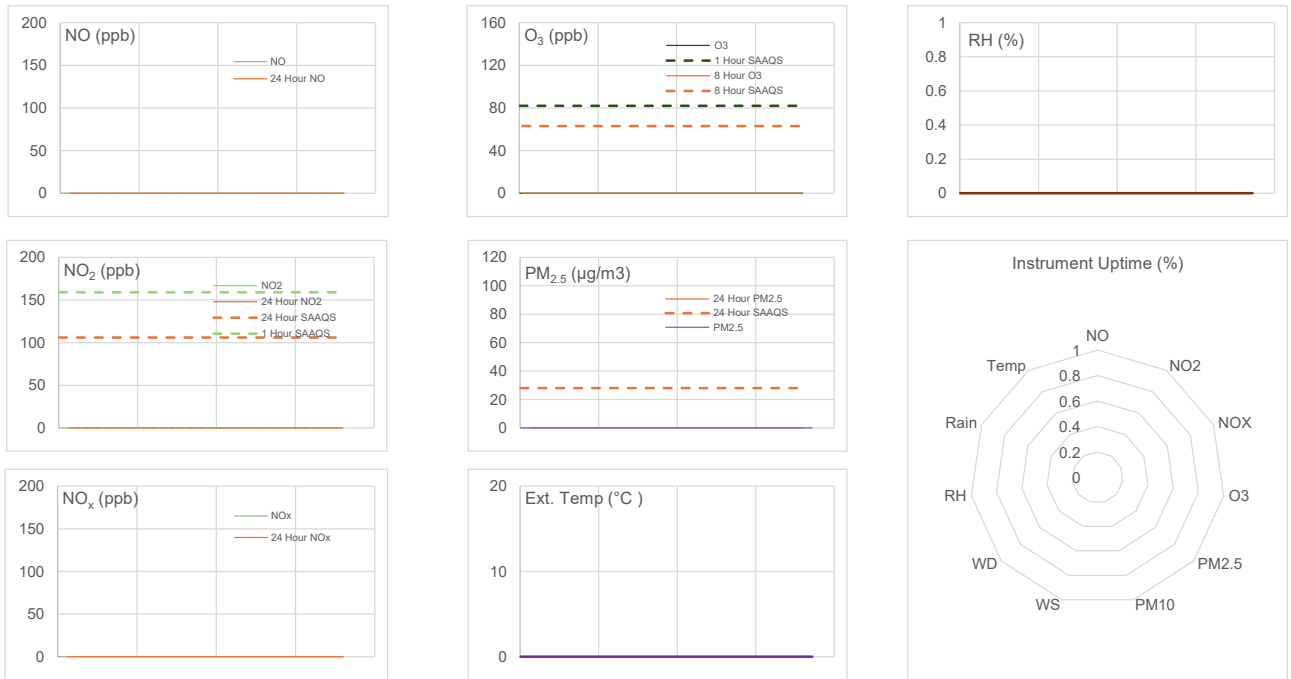


Exceedance Summary										
24-hour Exceedance Information			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	Precip.	NO	NO ₂	NO _x	O ₃	PM _{2.5}


SESAA Esterhazy Station - March 2026 Summary Report




Wind Rose



Pollution Rose NO₂



Pollution Rose O₃



Pollution Rose PM_{2.5}

Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class					
Wind Speed	m/s	NA	NA	NA	NA	NA	NA
NO ₂	ppb	NA	NA	NA	NA	NA	NA
O ₃	ppb	NA	NA	NA	NA	NA	NA
PM _{2.5}	µg/m ³	NA	NA	NA	NA	NA	NA

Monthly Update










- * All compliance parameters were less than 90% operational for the month.
- * The Airpointer system went offline on January 26, 2026, due to a power issue.
- * Quarterly calibrations completed on December 5, 2025



SESAA Glen Ewen Station - March 2026 Summary Report

Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
NO	ppb	No Data	0.0%	0.0	-	-	-	No Data	0	-	-
NO ₂	ppb	No Data	0.0%	0.0	-	106	0	No Data	0	159	-
NO _x	ppb	No Data	0.0%	0.0	-	-	-	No Data	0	-	-
SO ₂	ppb	No Data	0.0%	0.0	-	48	0	No Data	0	172	0
H ₂ S	ppb	No Data	0.0%	0.0	-	3.6	0	No Data	0	11	0
O ₃	ppb	No Data	0.0%	0.0	-	63 (8 hours)	0	No Data	0	82	0

SAAQS: Saskatchewan Ambient Air Quality Standards

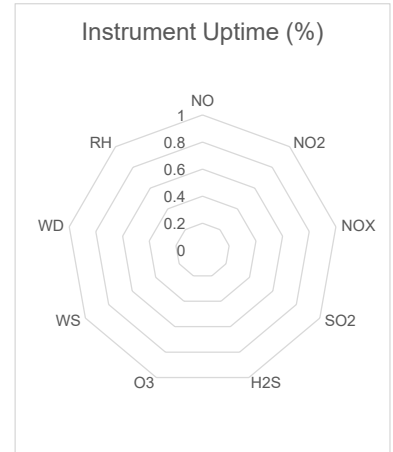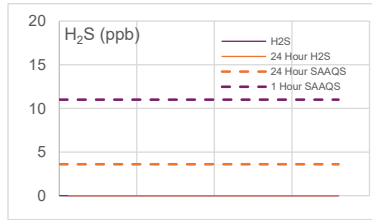


SESAA Glen Ewen Station - March 2026 Summary Report

Exceedance Summary (24-Hour Average)


24-hour Exceedance Information			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	H ₂ S	NO	NO ₂	NO _x	SO ₂	O ₃

Exceedance Summary (1-Hour Average)


1-hour Exceedance Information			Summary of Other Parameters During Exceedance					
Pollutant	Date and Time	Conc.	WS	WD	Precip.	SO ₂	NO ₂	O ₃




Wind Rose




NO₂ Pollution Rose



SO₂ Pollution Rose



H₂S Pollution Rose



O₃ Pollution Rose

Parameters	Unit	Color Code for Wind Speed and Pollutant Conc. Class							
Wind Speed	m/s	NA	NA	NA	NA	NA	NA	NA	NA
NO ₂	ppb	NA	NA	NA	NA	NA	NA	NA	NA
SO ₂	ppb	NA	NA	NA	NA	NA	NA	NA	NA
H ₂ S	ppb	NA	NA	NA	NA	NA	NA	NA	NA
O ₃	ppb	NA	NA	NA	NA	NA	NA	NA	NA

Monthly Update


- * All compliance parameters were less than 90% operational for the month.
- * Communication was lost with the Airpointer due to power issues on February 9, 2026
- * Quarterly calibrations were completed on November 30, 2025.











SESAA Oxbow Station - March 2026 Summary Report

Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
NO	ppb	0.1	94.6%	0.3	3/8/2026	-	-	2.3	03/02/2026 10:00	-	-
NO ₂	ppb	1.3	94.6%	2.8	3/2/2026	106	0	5.7	03/02/2026 08:00	159	0
NO _x	ppb	0.9	94.6%	2.7	3/2/2026	-	-	6.8	03/02/2026 09:00	-	-
SO ₂	ppb	1.4	94.6%	2.8	3/20/2026	48	0	7.4	03/08/2026 13:00	172	0
H ₂ S	ppb	0.6	94.6%	1.0	3/20/2026	3.6	0	1.2	03/20/2026 22:00	11	0
PM _{2.5}	µg/m ³	5.5	6.6%	6.8	3/2/2026	28	0	18.3	03/01/2026 13:00	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards




*If AQHI cannot be calculated due to missing parameters, AQHI plus is reported using PM_{2.5}

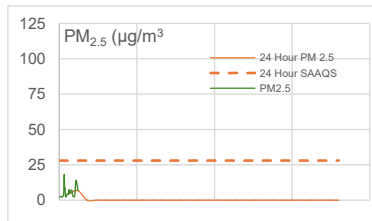

SESAA Oxbow Station - March 2026 Summary Report

Exceedance Summary

Exceedance Information			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	H ₂ S	NO	NO ₂	NO _x	SO ₂	PM _{2.5}



Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class						
Wind Speed	m/s	0.5 -W- 1.2	1.2 -W- 2.4	2.4 -W- 3.6	3.6 -W- 4.8	4.8 -W- 6.0	W > 6.0	
NO ₂	ppb	0.0-C- 1.2	1.2 -C- 2.4	2.4-C- 3.6	3.6-C- 4.8	4.8 -C- 6.0	C > 6.0	
SO ₂	ppb	0.0-C-2.0	2.0-C-4.0	4.0-C-6.0	6.0-C-8.0	8.0-C-10.0	C > 10.0	
H ₂ S	ppb	0.0-C-2.0	2.0-C-4.0	4.0-C-6.0	6.0-C-8.0	8.0-C-10.0	C > 10.0	
PM _{2.5}	µg/m ³	0.0-C-4.0	4.0-C-8.0	8.0-C-12.0	12.0-C-16.0	16.0-C-20.0	C > 20.0	

Monthly Update


- * All data has been zero drift and baseline corrected, when required. Data may change after final validation process.
- * All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
- * All compliance parameters were more than 90% operational for the month, except for PM_{2.5}
- * A total of 695 hours of PM_{2.5} data intermittent throughout the month were flagged as "analyzer malfunction," resulting in missing and flatlined data.
- * One hour of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
- * NO_x and SO₂ permeation tubes were depleted and replaced on March 28, 2026; therefore, daily span checks were not available and were not included in the data validation process.
- * Quarterly calibrations were completed on March 28, 2026.











SESAA Stoughton Station - March 2026 Summary Report

Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
NO	ppb	0.7	88.4%	2.0	3/13/2026	-	-	15.6	03/13/2026 15:00	-	-
NO ₂	ppb	0.8	88.4%	1.9	3/16/2026	106	0	11.6	03/13/2026 15:00	159	0
NO _x	ppb	1.1	88.4%	3.4	3/2/2026	-	-	27.2	03/13/2026 15:00	-	0
SO ₂	ppb	1.2	94.9%	3.9	3/13/2026	48	0	25.6	03/13/2026 15:00	172	0
H ₂ S	ppb	1.7	94.8%	2.7	3/23/2026	3.6	0	3.3	03/22/2026 22:00	11	0
PM _{2.5}	µg/m ³	5.7	38.3%	13.4	3/3/2026	28	0	26.7	-	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards

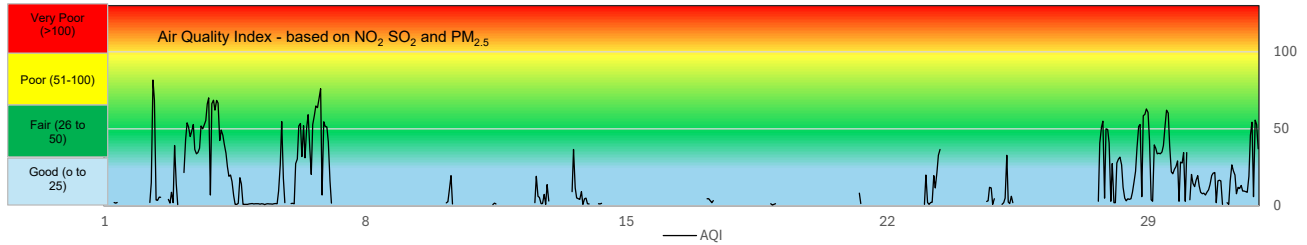








*If AQHI cannot be calculated due to missing parameters, AQHI plus is reported using PM_{2.5}



SESAA Torquay Station - March 2026 Summary Report


Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
SO ₂	ppb	1.3	94.9%	2.2	3/4/2026	48	0	7.7	03/28/2026 16:00	172	0
H ₂ S	ppb	0.8	95.0%	1.6	3/29/2026	3.6	0	1.8	03/29/2026 19:00	11	0
PM _{2.5}	µg/m ³	4.8	100.0%	11.3	3/3/2026	28	0	24.3	03/25/2026 08:00	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards

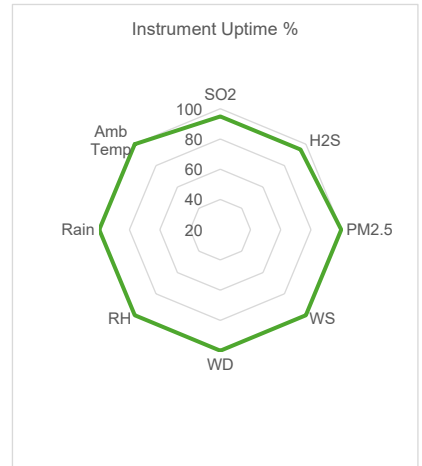


Exceedance Summary								
24-hour Exceedance Information			Summary of other Parameters during Exceedance					
Pollutant	Date	Conc.	WS	WD	Precip.	SO ₂	H ₂ S	PM _{2.5}


SESAA Torquay Station - March 2026 Summary Report




Wind Rose



Pollution Rose SO₂



Pollution Rose H₂S



Pollution Rose PM_{2.5}

Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class						
Wind Speed	m/s	0.5 -W- 1.2	1.2 -W- 2.4	2.4 -W- 3.6	3.6 -W- 4.8	4.8 -W- 6.0	W > 6.0	
SO ₂	ppb	0.0-C-0.6	0.6-C-1.2	1.2-C-1.8	1.8-C-2.4	2.4-C-3.0	C > 3.0	
H ₂ S	ppb	0.0-C-0.6	0.6-C-1.2	1.2-C-1.8	1.8-C-2.4	2.4-C-3.0	C > 3.0	
PM _{2.5}	µg/m ³	0.0-C-4.0	4.0-C-8.0	8.0-C-12.0	12.0-C-16.0	16.0-C-20.0	C > 20.0	

Monthly Update








- * All data has been zero drift and baseline corrected, where required. Data may change after final validation process.
- * All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
- * All compliance parameters were more than 90% operational for the month.
- * One hour of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
- * H₂S permeation tube was depleted and replaced on March 31, 2026; therefore, daily span checks were not available and were not included in the data validation process.
- * Most recent quarterly calibrations were completed on March 30 and 31, 2026.



SESAA Wauchope Station - March 2026 Summary Report

Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
SO ₂	ppb	0.3	6.9%	0.4	3/30/2026	48	0	1	03/29/2026 24:00	172	0
H ₂ S	ppb	0.1	6.9%	0.1	3/31/2026	3.6	0	0.5	03/29/2026 23:00	11	0
PM _{2.5}	µg/m ³	14.5	99.3%	59.9	3/27/2026	28	3	125.7	03/28/2026 05:00	-	-

SAAQS: Saskatchewan Ambient Air Quality Standards




Exceedance Summary (24-Hour Average)

24-hour Exceedance Information			Summary of other Parameters during Exceedance						
Pollutant	Date	Conc.	WS	WD	Precip.	SO ₂	H ₂ S	PM _{2.5}	
PM _{2.5}	26-Mar	33.5	<Samp	<Samp	<Samp	<Samp	<Samp	33.5	
PM _{2.5}	27-Mar	59.9	<Samp	<Samp	<Samp	<Samp	<Samp	59.9	
PM _{2.5}	28-Mar	54.1	<Samp	<Samp	<Samp	<Samp	<Samp	54.1	


SESAA Wauchope Station - March 2026 Summary Report

Exceedance Summary (1-Hour Average)


1-hour Exceedance Information			Summary of Other Parameters During Exceedance					
Pollutant	Date and Time	Conc.	WS	WD	Precip.	SO ₂	H ₂ S	PM _{2.5}




Wind Rose



Pollution Rose SO₂



Pollution Rose H₂S



Pollution Rose PM_{2.5}

Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class						
Wind Speed	m/s	N/A	N/A	N/A	N/A	N/A	N/A	N/A
SO ₂	ppb	0.0-C-0.6	0.6-C-1.2	1.2-C-1.8	1.8-C-2.4	2.4-C-3.0	C > 3.0	
H ₂ S	ppb	0.0-C-0.6	0.6-C-1.2	1.2-C-1.8	1.8-C-2.4	2.4-C-3.0	C > 3.0	
PM _{2.5}	µg/m ³	0.0-C-4.0	4.0-C-8.0	8.0-C-12.0	12.0-C-16.0	16.0-C-20.0	C > 20.0	

Monthly Update

- * All data has been zero baseline corrected, when required. Data may change after final validation process.
- * All compliance parameters were within the Saskatchewan Ambient Air Quality Standards with the exception of three 24-hour PM_{2.5} exceedances.
- * All compliance parameters were less 90% operational for the month with the exception of PM_{2.5}.
- * A total of 744 hours of data flagged as "analyzer failure" for WS/WD
- * A total of 693 hours of data flagged as analyzer malfunctioning for H₂S and SO₂.
- * H₂S and SO₂ analyzers were installed back on March 29, 2026.
- * PM_{2.5} data appears to be noisy from March 26, 2026 & requires investigation. The data has been retained for reference & appropriately flagged.
- * One hour of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
- * Pollution Rose data developed using wind data from the nearby Oxbow Station.





SESAA Weyburn Station - March 2026 Summary Report

Exceedance Summary (24-Hours Average)

24-hours Exceedance Information			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	H ₂ S	NO	NO ₂	NOx	SO ₂	PM _{2.5}

Exceedance Summary (1-Hour Average)

1-hour Exceedance Information			Summary of Other Parameters During Exceedance					
Pollutant	Date and Time	Conc.	WS	WD	Precip.	SO ₂	NO ₂	PM _{2.5}
H ₂ S	03/07/2026 07:00	30.0	1.27	163.1	0.0	1.6	0.8	NoData

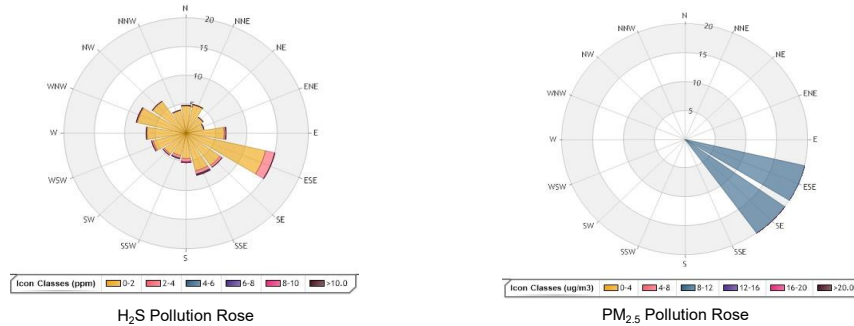

Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class						
Wind Speed	m/s	0.5-W-1.2	1.2-W-2.4	2.4-W-3.6	3.6-W-4.8	4.8-W-6.0	W > 6.0	
NO ₂	ppb	0.0-C-1.2	1.2-C-2.4	2.4-C-3.6	3.6-C-4.8	4.8-C-6.0	C > 6.0	
SO ₂	ppb	0.0-C-2.0	2.0-C-4.0	4.0-C-6.0	6.0-C-8.0	8.0-C-10.0	C > 10.0	
H ₂ S	ppb	0.0-C-2.0	2.0-C-4.0	4.0-C-6.0	6.0-C-8.0	8.0-C-10.0	C > 10.0	
PM _{2.5}	µg/m ³	0.0-C-4.0	4.0-C-8.0	8.0-C-12.0	12.0-C-16.0	16.0-C-20.0	C > 20.0	

Monthly Update

- * All data has been zero drift and baseline corrected, where required. Data may change after final validation process.
- * All compliance parameters were within the Saskatchewan Ambient Air Quality Standards except for one, one-hour H₂S exceedance.
- * All compliance parameters were more than 90% operational for the month with the exception of PM_{2.5}.
- * A total of 736 hours of PM_{2.5} data was flagged as "analyzer error," resulting in missing and flatlined data.
- * One hour of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
- * The SO₂ and NO₂ permeation tube was depleted, and as a result, daily span checks were not included in the data process.
- * Most recent quarterly calibrations were completed on April 1, 2025.

