

SESAA Esterhazy Station - September 2026 Summary Report


Pollutant		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Concentration	Date and Time		
NO	ppb	0.6	75.0%	1.0	9/24/2026	-	-	5.2	09/21/2026 07:00	-	-
NO_2	ppb	1.4	75.0%	4.4	9/24/2026	106	0	20.3	09/24/2026 19:00	159	0
NO_x	ppb	2.0	75.0%	5.5	9/24/2026	-	-	24.5	09/24/2026 19:00	-	-
O_3	ppb	15.1	60.1%	29.8	9/10/2026	63 (8-Hrs Rolling Avg)	0	30.4	09/22/2026 17:00	82	0
$PM_{2.5}$	$\mu g/m^3$	5.1	82.1%	9.7	9/19/2026	28	0	26.9	09/27/2026 21:00	-	-


SAAQS: Saskatchewan Ambient Air Quality Standards

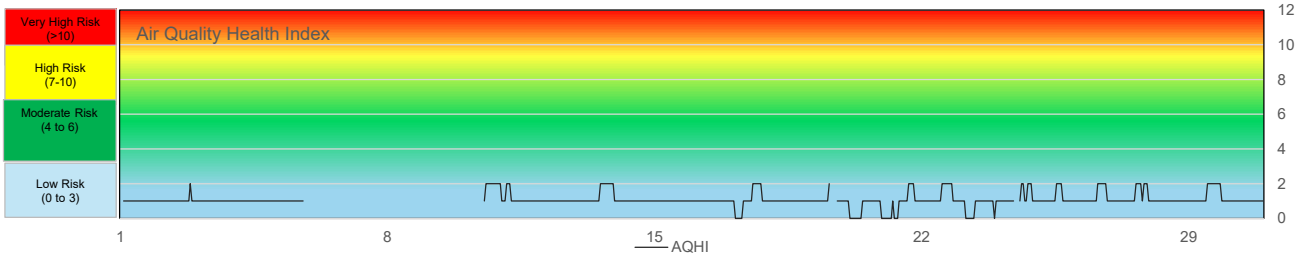



*If AQHI cannot be calculated due to missing parameters, AQHI plus is reported using $PM_{2.5}$

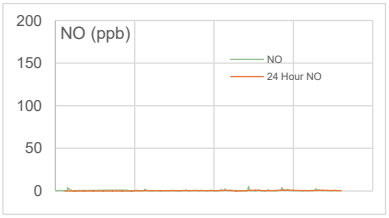


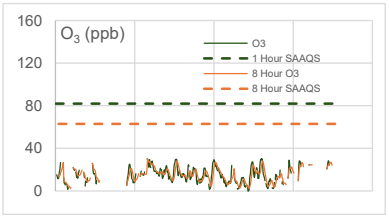


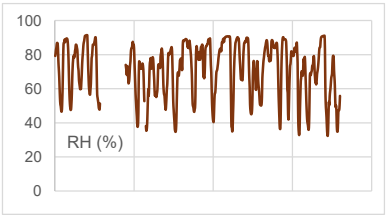


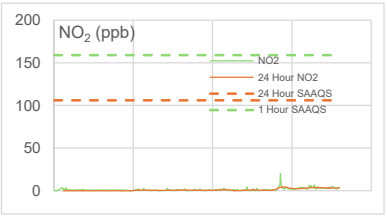

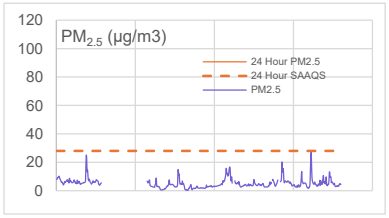

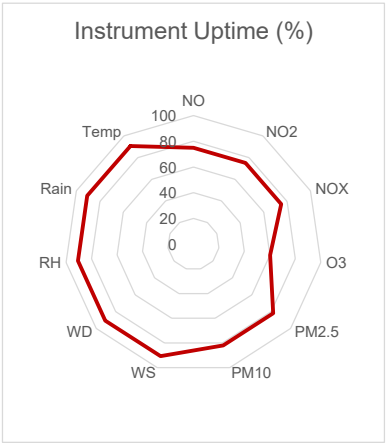

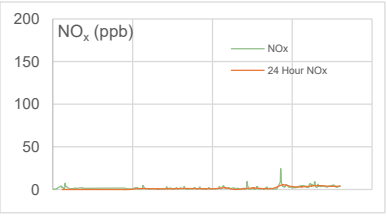

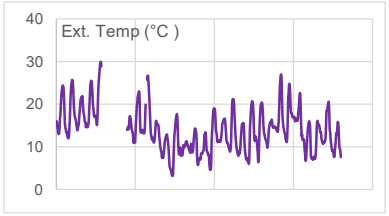


Exceedance Summary (24-Hour Average)

			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	Precip.	NO	NO_2	NOx	O_3	$PM_{2.5}$


Exceedance Summary (1-hour Average)

			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	Precip.	NO	NO_2	NOx	O_3	$PM_{2.5}$


SESAA Esterhazy Station - September 2026 Summary Report

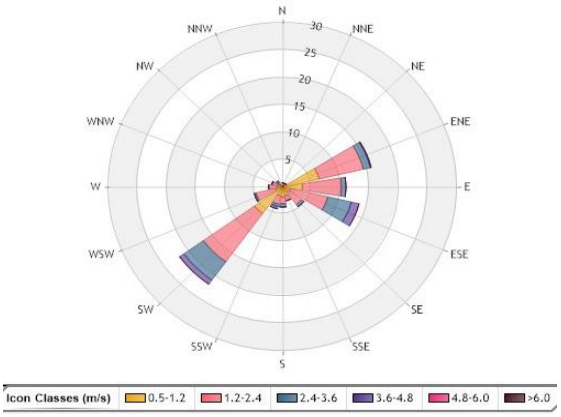


Wind Rose

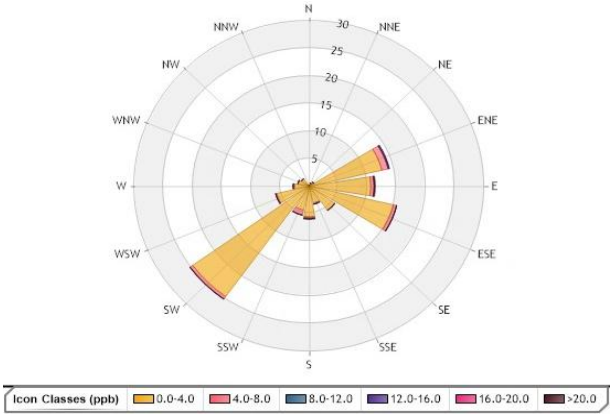

Pollution Rose NO_2

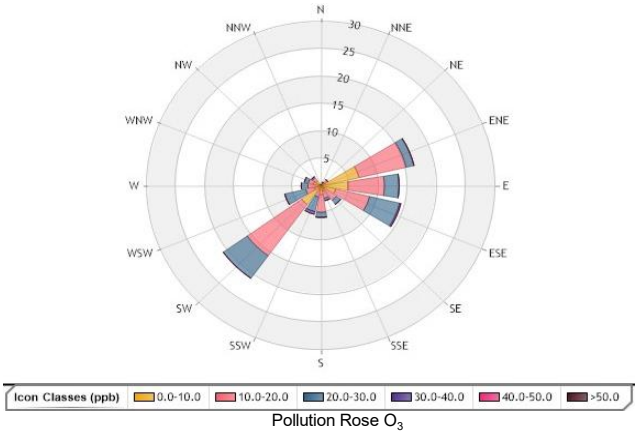

Pollution Rose O_3

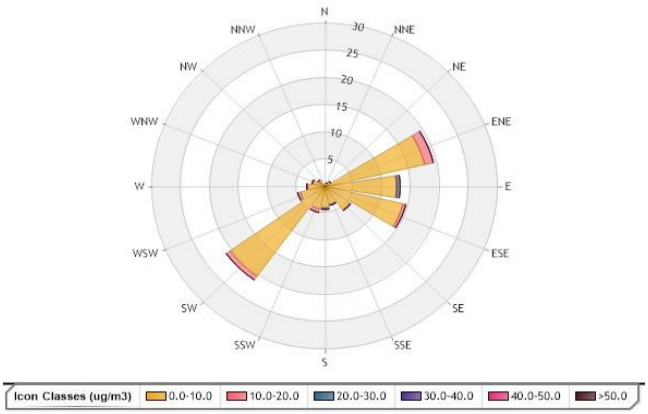

Pollution Rose $PM_{2.5}$

Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class					
Wind Speed	m/s	0.5 - 1.2	1.2 - 2.4	2.4 - 3.6	3.6 -4.8	4.8 - 6.0	C> 6.0
NO_2	ppb	0.0-C-4.0	4.0-C-8.0	8.0-C-12.0	12.0-C-16.0	16.0-C-20.0	C> 20.0
O_3	ppb	0.0-C-10.0	10.0-C-20.0	20.0-C-30.0	30.0-C-40.0	40.0-C-50.0	C> 50.0
$PM_{2.5}$	µg/m^3	0.0-C-10.0	10.0-C-20.0	20.0-C-30.0	30.0-C-40.0	40.0-C-50.0	C> 50.0


Monthly Update


* All data has been zero drift, and baseline corrected, when required. Data may change after final validation process.
* All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
* All compliance parameters were less than 90% operational for the month.
* A total of 287 hours of O_3 data was unavailable due to analyzer error and power issues.
* A total of 129 hours of $PM_{2.5}$ data was unavailable due to analyzer error and power issues.
* A total of 80 hours of NO_2 data was unavailable due to analyzer error as well as power issues.
* Shelter temperatures fluctuated between 23°C and 47.5°C. High temperatures may have impacted instrument performance & data quality, and the instrument was shut down. Consequently the data are considered qualitative and available for reference only.
* Quarterly calibrations completed on September 24, 2026


SESAA Glen Ewen Station - September 2026 Summary Report


Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
NO	ppb	1.1	72.8%	2.3	9/3/2026	-	-	17.3	09/03/2026 10:00	-	-
NO_2	ppb	0.7	72.8%	1.3	9/30/2026	106	0	5.9	09/01/2026 22:00	159	0
NO_x	ppb	1.6	72.8%	2.9	9/3/2026	-	-	19.4	09/03/2026 10:00	-	-
SO_2	ppb	0.1	94.6%	0.5	9/30/2026	48	0	3.2	09/13/2026 10:00	172	0
H_2S	ppb	0.3	94.6%	1.0	9/13/2026	3.6	0	6.1	09/03/2026 10:00	11	0
O_3	ppb	19.7	94.4%	38.0	9/5/2026	63 (8 hrs rolling avg)	0	42.2	09/10/2026 16:00	82	0


SAAQS: Saskatchewan Ambient Air Quality Standards

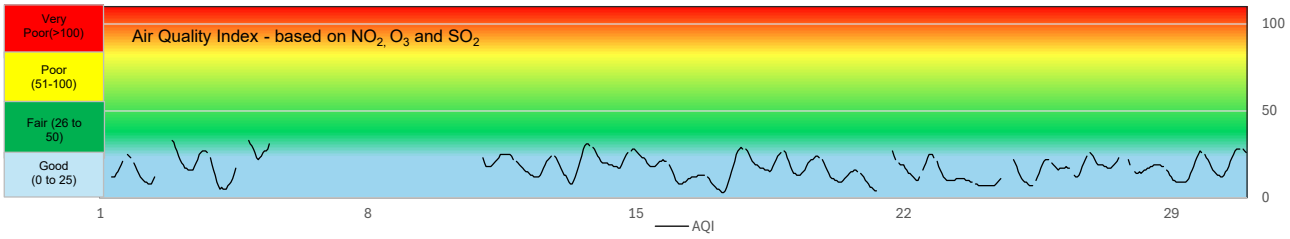


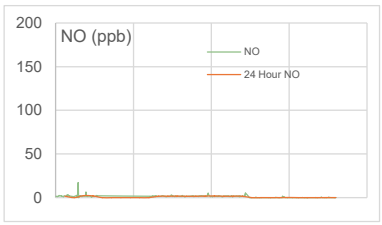


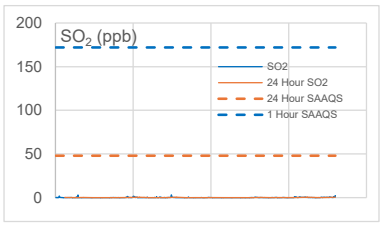


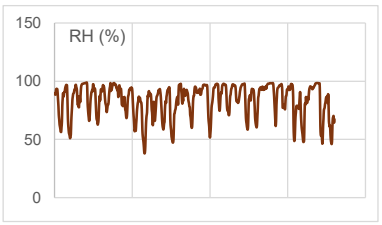


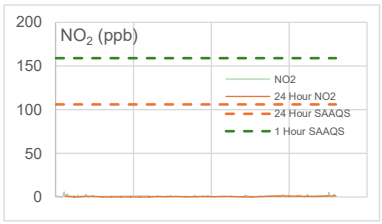

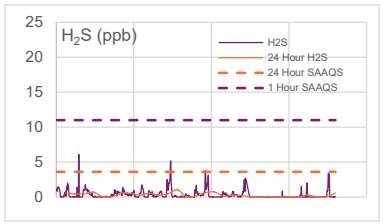

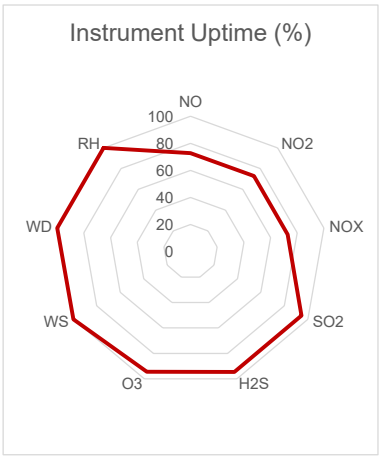

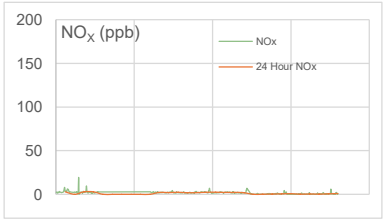


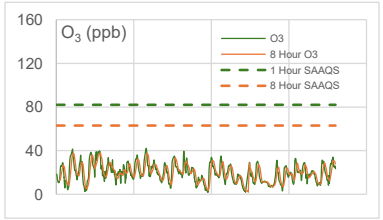


SESAA Glen Ewen Station - September 2026 Summary Report

Exceedance Summary (24-Hour Average)											
24-hour Exceedance Information			Summary of other Parameters during Exceedance								
Pollutant	Date	Conc.	WS	WD	NO	NO_2	NOx	SO_2	H_2S	O_3


Exceedance Summary (1-Hour Average)								
1-hour Exceedance Information			Summary of Other Parameters During Exceedance					
Pollutant	Date and Time	Conc.	WS	WD	Precip.	SO_2	NO_2	O_3

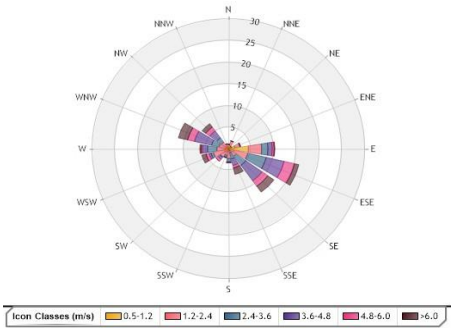


Wind Rose

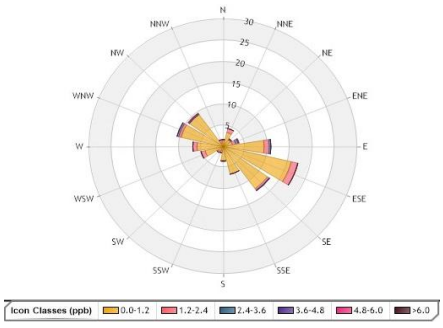


NO_2 Pollution Rose

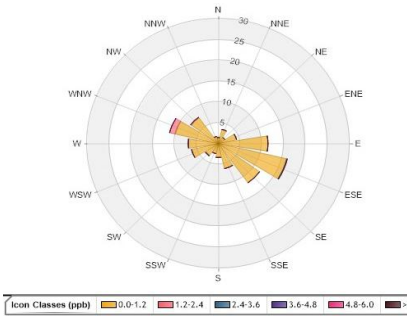

SO_2 Pollution Rose

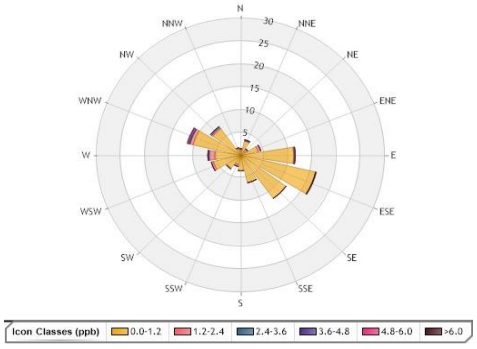

H_2S Pollution Rose

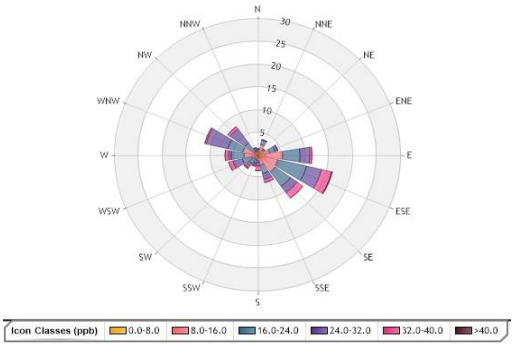

O_3 Pollution Rose

Parameters	Unit	Color Code for Wind Speed and Pollutant Conc. Class					
Wind Speed	m/s	0.5-W- 1.2	1.2 -W- 2.4	2.4 -W- 3.6	3.6 -W- 4.8	4.8 -W- 6.0	W > 6.0
NO_2	ppb	0.0-C- 1.2	1.2 -C- 2.4	2.4 -C- 3.6	3.6 -C- 4.8	4.8 -C- 6.0	C > 6.0
SO_2	ppb	0.0-C- 1.2	1.2 -C- 2.4	2.4 -C- 3.6	3.6 -C- 4.8	4.8 -C- 6.0	C > 6.0
H_2S	ppb	0.0-C- 1.2	1.2 -C- 2.4	2.4 -C- 3.6	3.6 -C- 4.8	4.8 -C- 6.0	C > 6.0
O_3	ppb	0.0-C-8.0	8.0-C-16.0	16.0-C-24.0	24.0-C-32.0	32.0-C-40.0	C > 40.0


Monthly Update

* All data has been zero drift and baseline corrected, when required. Data may change after final validation process.
* All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
* All compliance parameters were more than 90% operational for the month with the exception of NOx.
* A total of 196 hours of NO_2 data unavailable due to analyzer error.
* One hour of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
* Shelter temperature instability during the reporting period affected analyzers internal checks and performance, resulting in intermittent data loss and compromising quality of data.
* Quarterly calibrations were completed on September 21, 2026.


SESAA Oxbow Station - September 2026 Summary Report


Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
NO	ppb	0	94.7%	0.1	9/17/2026	-	-	1.2	09/17/2026 02:00	-	-
NO_2	ppb	4.8	94.7%	7.4	9/29/2026	106	0	11.1	09/27/2026 22:00	159	0
NO_x	ppb	4.4	94.7%	7.3	9/29/2026	-	-	10.7	09/27/2026 22:00	-	-
SO_2	ppb	0.3	95.0%	0.6	9/20/2026	48	0	3.5	09/27/2026 03:00	172	0
H_2S	ppb	1.0	95.0%	1.4	9/10/2026	3.6	0	3.0	09/10/2026 07:00	11	0
$PM_{2.5}$	$\mu g/m^3$	6	92.1%	8.7	9/10/2026	28	0	61.7	09/22/2026 13:00	-	-


SAAQS: Saskatchewan Ambient Air Quality Standards

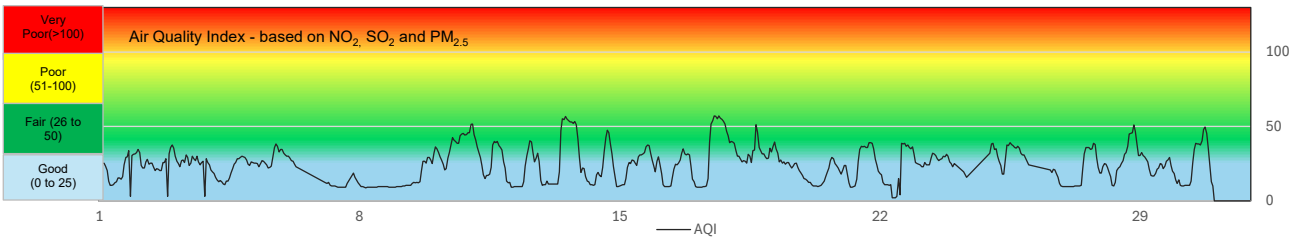



*If AQHI cannot be calculated due to missing parameters, AQHI plus is reported using $PM_{2.5}$

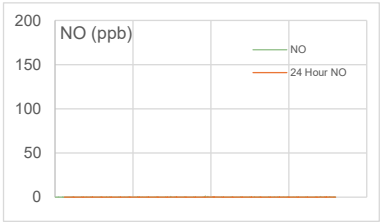


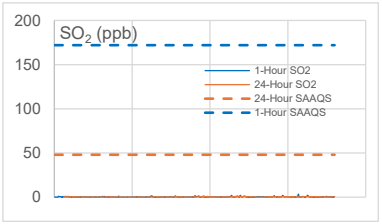


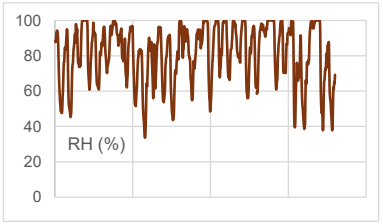


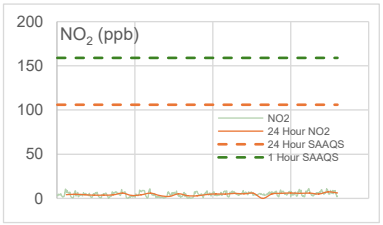

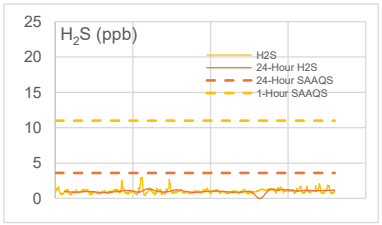

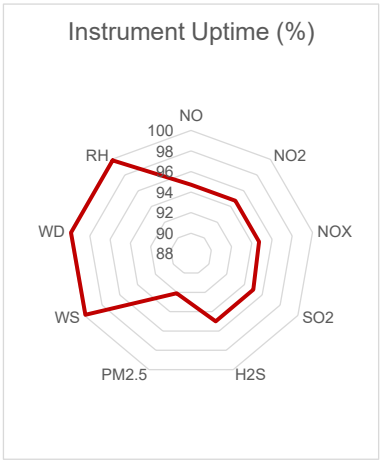

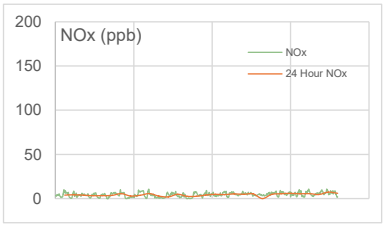


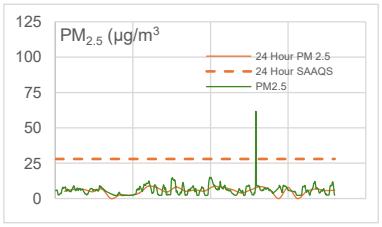


SESAA Oxbow Station - September 2026 Summary Report

Exceedance Summary


Exceedance Information			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	H_2S	NO	NO_2	NOx	SO_2	$PM_{2.5}$

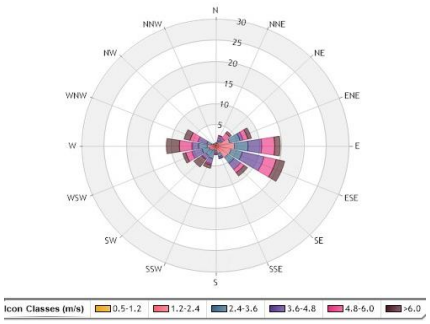


Wind Rose

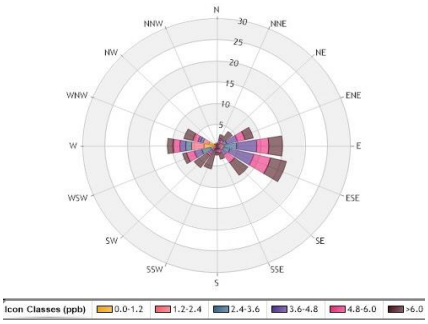


NO_2 Pollution Rose

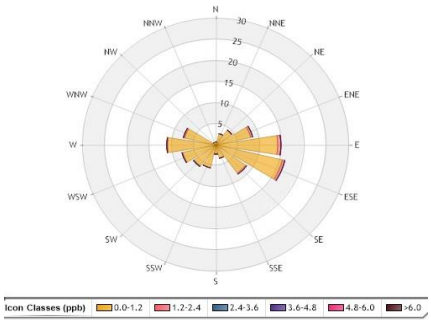

SO_2 Pollution Rose

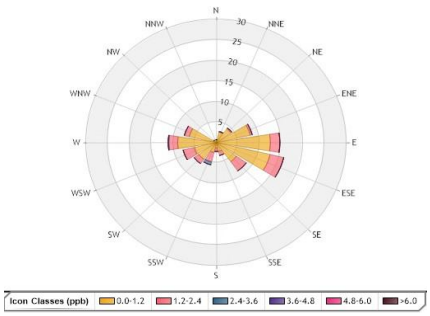

H_2S Pollution Rose

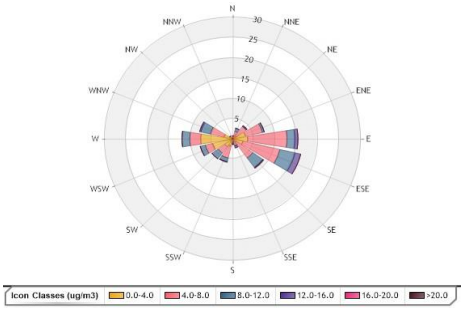

$PM_{2.5}$ Pollution Rose

Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class					
Wind Speed	m/s	0.5 -W- 1.2	1.2 -W- 2.4	2.4 -W- 3.6	3.6 -W- 4.8	4.8 -W- 6.0	W > 6.0
NO_2	ppb	0.0-C- 1.2	1.2 -C- 2.4	2.4-C- 3.6	3.6-C- 4.8	4.8 -C- 6.0	C > 6.0
SO_2	ppb	0.0-C-2.0	2.0-C-4.0	4.0-C-6.0	6.0-C-8.0	8.0-C-10.0	C > 10.0
H_2S	ppb	0.0-C-2.0	2.0-C-4.0	4.0-C-6.0	6.0-C-8.0	8.0-C-10.0	C > 10.0
$PM_{2.5}$	$\mu g/m^3$	0.0-C-4.0	4.0-C-8.0	8.0-C-12.0	12.0-C-16.0	16.0-C-20.0	C > 20.0


Monthly Update

* All data has been zero drift and baseline corrected, when required. Data may change after final validation process.
* All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
* All compliance parameters were more than 90% operational for the month.
* One hour of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
* Quarterly calibrations were completed on September 23, 2026.


SESAA Stoughton Station - September 2026 Summary Report


Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
NO	ppb	0.1	94.7%	0.6	9/21/2026	-	-	4.3	09/02/2026 17:00	-	-
NO_2	ppb	0.7	94.7%	1.7	9/24/2026	106	0	5.0	09/27/2026 24:00	159	0
NO_x	ppb	0.7	94.7%	1.9	9/23/2026	-	-	5.6	09/21/2026 18:00	-	-
SO_2	ppb	0.3	94.7%	1.2	9/22/2026	48	0	4.4	09/25/2026 11:00	172	0
H_2S	ppb	0.7	94.7%	1.7	9/13/2026	3.6	0	6.1	09/16/2026 22:00	11	0
$PM_{2.5}$	$\mu g/m^3$	5.3	99.6%	7.5	9/2/2026	28	0	28.4	09/27/2026 21:00	-	-


SAAQS: Saskatchewan Ambient Air Quality Standards

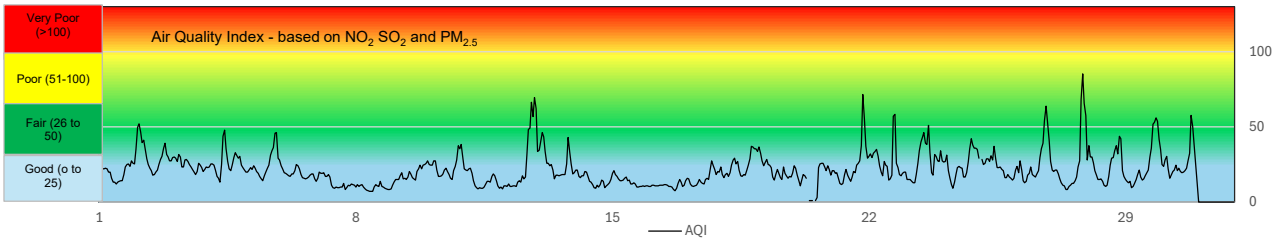



*If AQHI cannot be calculated due to missing parameters, AQHI plus is reported using $PM_{2.5}$

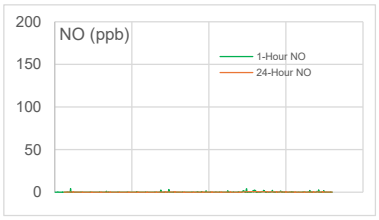


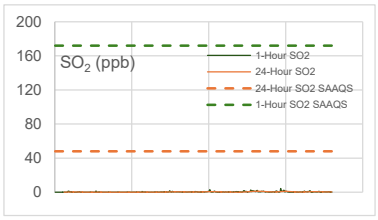


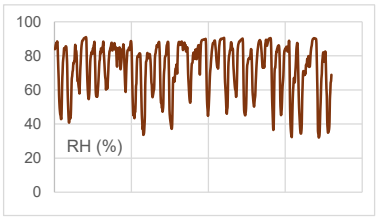


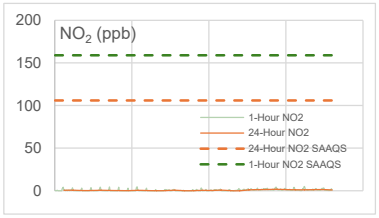

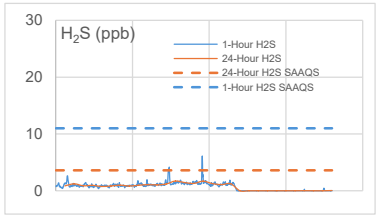

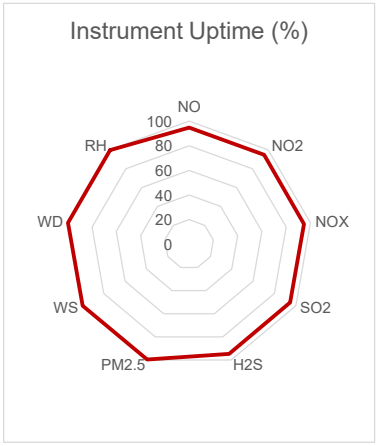

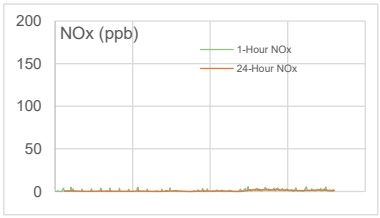


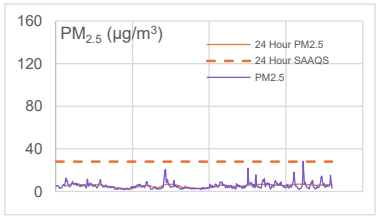


SESAA Stoughton Station - September 2026 Summary Report

Exceedance Summary (24-hour)										
Exceedance Summary			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	H_2S	NO	NO_2	NOx	SO_2	$PM_{2.5}$


Exceedance Summary (1-hour)										
Exceedance Summary			Summary of other Parameters during Exceedance							
Pollutant	Date & Time	Conc.	WS	WD	H_2S	NO	NO_2	NOx	SO_2	$PM_{2.5}$

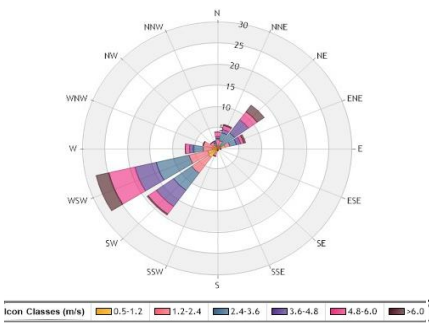


Wind Rose

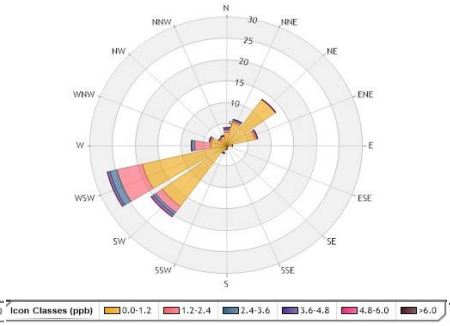


NO_2 Pollution Rose

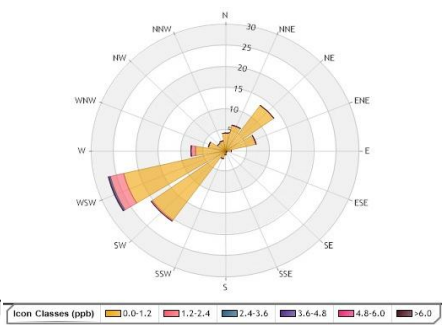

SO_2 Pollution Rose

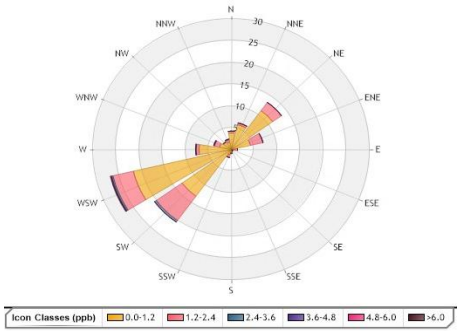

H_2S Pollution Rose

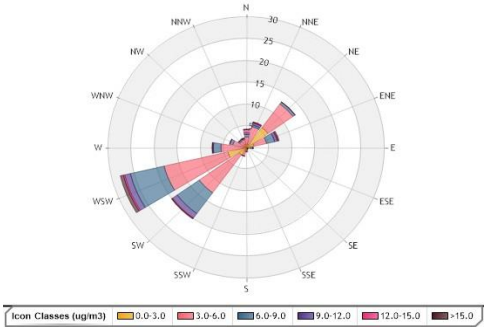

$PM_{2.5}$ Pollution Rose

Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class					
Wind Speed	m/s	0.5 -W- 1.2	1.2 -W- 2.4	2.4 -W- 3.6	3.6 -W- 4.8	4.8 -W- 6.0	W > 6.0
NO_2	ppb	0.0 -C- 1.2	1.2 -C- 2.4	2.4 -C- 3.6	3.6 -C- 4.8	4.8 -C- 6.0	C > 6.0
SO_2	ppb	0.0 -C- 1.2	1.2 -C- 2.4	2.4 -C- 3.6	3.6 -C- 4.8	4.8 -C- 6.0	C > 6.0
H_2S	ppb	0.0 -C- 1.2	1.2 -C- 2.4	2.4 -C- 3.6	3.6 -C- 4.8	4.8 -C- 6.0	C > 6.0
$PM_{2.5}$	µg/m^3	0.0-C-3.0	3.0-C-6.0	6.0-C-9.0	9.0-C-12.0	12.0-C-15.0	C > 15.0


Monthly Update


* All data has been zero drift and baseline corrected, if needed. Data may change after final validation process.
* All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
* All compliance parameters were over 90% operational for the month.
* One hour of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
* Quarterly calibrations were completed on September 20, 2026.


SESAA Torquay Station - September 2026 Summary Report


Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
SO_2	ppb	0.7	92.6%	1.7	9/4/2026	48	0	5.6	09/04/2026 19:00	172	0
H_2S	ppb	1.2	93.2%	2.0	9/5/2026	3.6	0	5.7	09/07/2026 05:00	11	0
$PM_{2.5}$	µg/m^3	6.5	99.9%	24.4	9/2/2026	28	0	90.7	09/02/2026 16:00	-	-


SAAQS: Saskatchewan Ambient Air Quality Standards

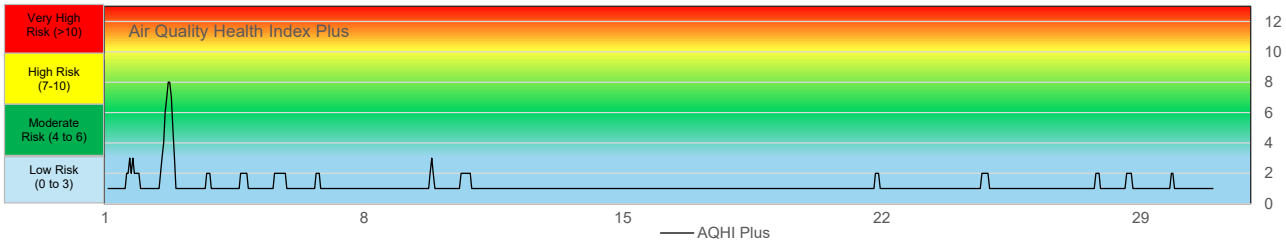


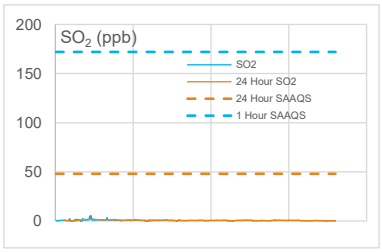


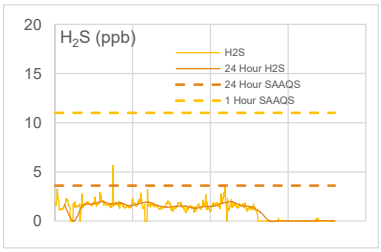

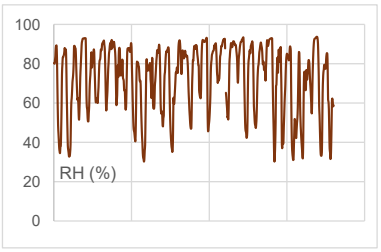

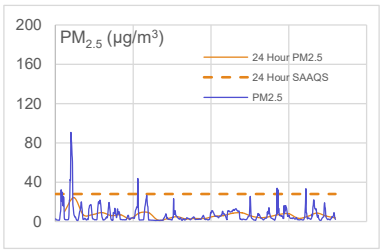


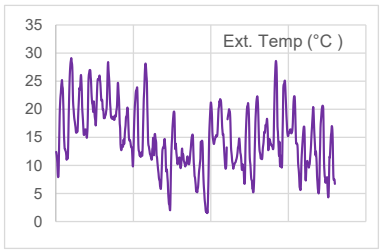

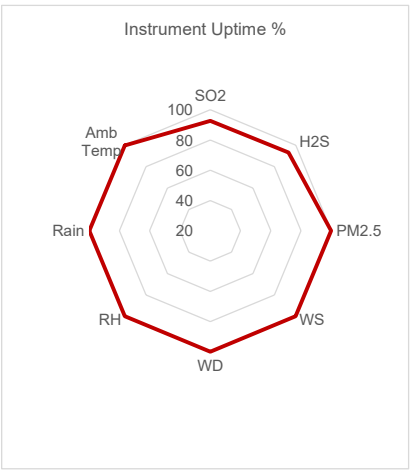


Exceedance Summary								
24-hour Exceedance Information			Summary of other Parameters during Exceedance					
Pollutant	Date	Conc.	WS	WD	Precip.	SO_2	H_2S	$PM_{2.5}$


SESAA Torquay Station - September 2026 Summary Report

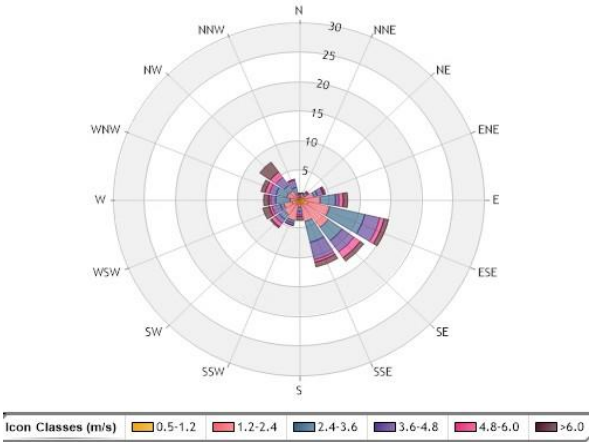


Wind Rose

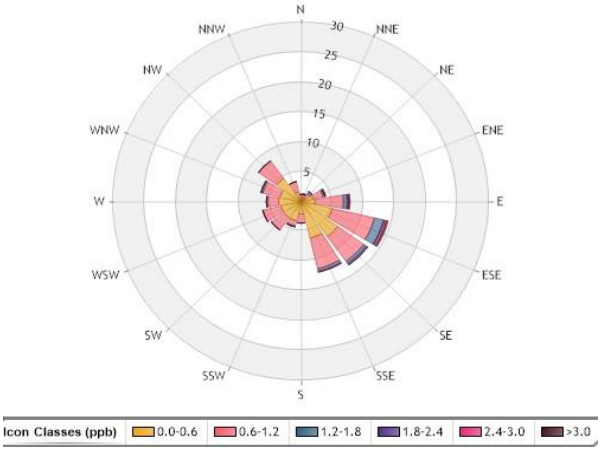

Pollution Rose SO_2

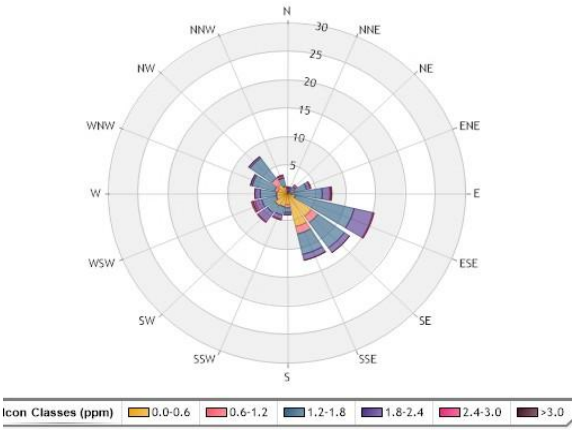

Pollution Rose H_2S

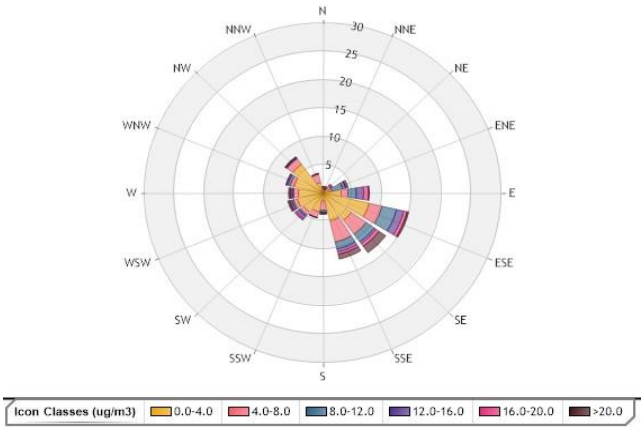

Pollution Rose $PM_{2.5}$

Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class					
Wind Speed	m/s	0.5 -W- 1.2	1.2 -W- 2.4	2.4 -W- 3.6	3.6 -W- 4.8	4.8 -W- 6.0	W > 6.0
SO_2	ppb	0.0-C-0.6	0.6-C-1.2	1.2-C-1.8	1.8-C-2.4	2.4-C-3.0	C > 3.0
H_2S	ppb	0.0-C-0.6	0.6-C-1.2	1.2-C-1.8	1.8-C-2.4	2.4-C-3.0	C > 3.0
$PM_{2.5}$	µg/m^3	0.0-C-4.0	4.0-C-8.0	8.0-C-12.0	12.0-C-16.0	16.0-C-20.0	C > 20.0


Monthly Update


* All data has been zero drift and baseline corrected, where required. Data may change after final validation process.
* All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
* All compliance parameters were greater than 90% operational for the month.
* One hour of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
* Shelter temperature fluctuated during the reporting period and reached unusually high levels, potentially affecting data quality. The affected data were flagged and provided for reference only.
* Most recent quarterly calibrations were completed on September 22, 2026.


SESAA Wauchope Station - September 2026 Summary Report


Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
SO_2	ppb	0.7	36.8%	0.9	9/9/2026	48	0	1.6	09/05/2026 13:00	172	0
H_2S	ppb	1.5	36.8%	2.6	9/2/2026	3.6	0	7.2	09/02/2026 05:00	11	0
$PM_{2.5}$	$\mu g/m^3$	No Data	0.0%	0.0	NA	28	0	No Data	NA	-	-


SAAQS: Saskatchewan Ambient Air Quality Standards

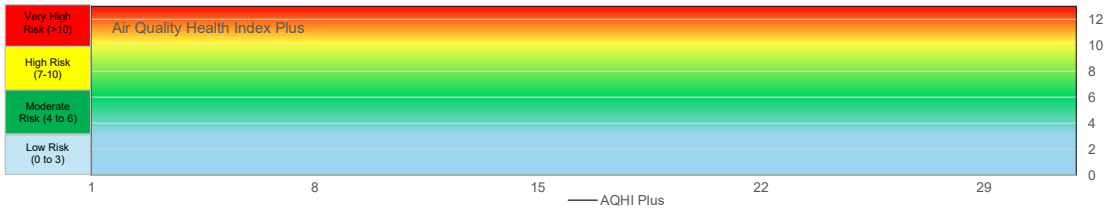


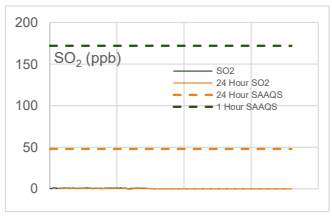


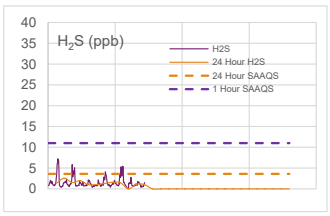

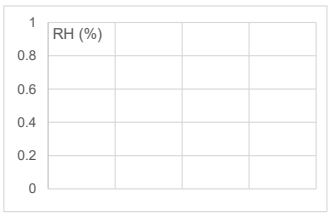

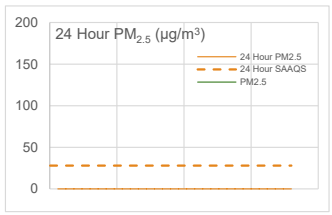

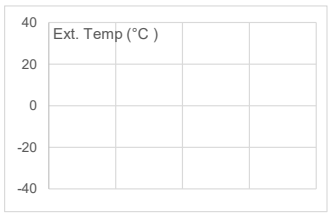


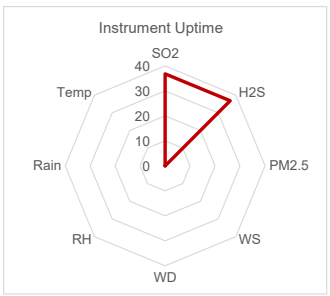


Exceedance Summary (24-Hour Average)								
24-hour Exceedance Information			Summary of other Parameters during Exceedance					
Pollutant	Date	Conc.	WS	WD	Precip.	SO_2	H_2S	$PM_{2.5}$

SESAA Wauchope Station - September 2026 Summary Report


Exceedance Summary (1-Hour Average)								
1-hour Exceedance Information			Summary of Other Parameters During Exceedance					
Pollutant	Date and Time	Conc.	WS	WD	Precip.	SO_2	H_2S	$PM_{2.5}$

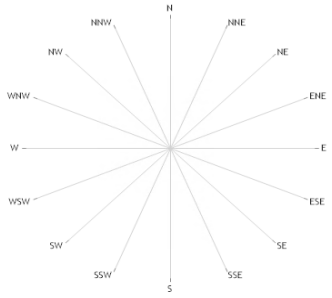


Wind Rose

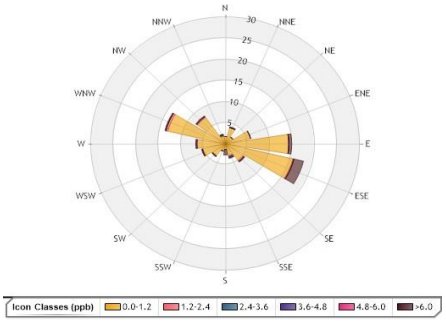

Pollution Rose SO_2

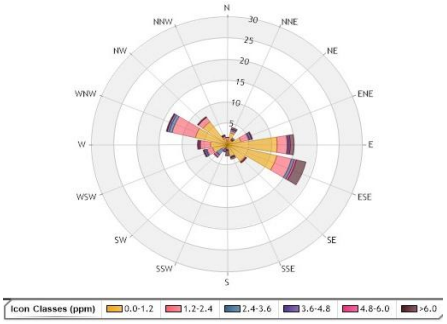

Pollution Rose H_2S

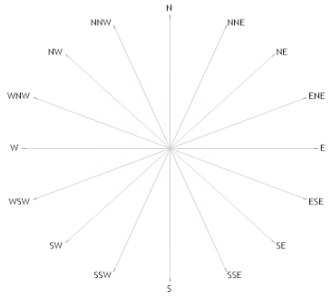

Pollution Rose $PM_{2.5}$

SESAA Wauchope Station - September 2026 Summary Report

Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class					
Wind Speed	m/s	N/A	N/A	N/A	N/A	N/A	N/A
SO_2	ppb	0.0-C-1.2	1.2-C-2.4	2.4-C-3.6	3.6-C-4.8	4.8-C-6.0	C > 6.0
H_2S	ppb	0.0-C-1.2	1.2-C-2.4	2.4-C-3.6	3.6-C-4.8	4.8-C-6.0	C > 6.0
$PM_{2.5}$	$\mu g/m^3$	N/A	N/A	N/A	N/A	N/A	N/A


Monthly Update

* All data has been zero baseline corrected, when required. Data may change after final validation process.
* All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
* All compliance parameters were less than 90% operational for the month.
* Meteorological sensor removed for repair.
* The $PM_{2.5}$ analyzer has been malfunctioning and no valid data are available. The instrument will be inspected during the next quarterly site visit.
* One hour of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
* H_2S and SO_2 analyzers were removed for repair on September 20, 2026, due to excessive noise and unstable readings. Data from September 13-19, 2026, were invalidated. Data prior to September 13 are considered reference only.
* Pollution Rose data developed using wind data from the nearby Glen Ewan Station.


SESAA Weyburn Station - September 2026 Summary Report


Pollutants		Month Records		24 Hour Records				1 Hour Records			
Name	Unit	Average Concentration	Uptime	Maximum		SAAQS*	Exceedance Days	Maximum		SAAQS*	Exceed Hours
				Conc.	Date			Conc.	Date and Time		
NO	ppb	0.3	95.0%	1.7	9/8/2026	-	-	29.6	09/08/2026 16:00	-	-
NO_2	ppb	0.3	95.0%	1.3	9/8/2026	106	0	26.6	09/08/2026 16:00	159	0
NO_x	ppb	0.4	95.0%	2.8	9/8/2026	-	-	56.1	09/08/2026 16:00	-	-
SO_2	ppb	2.4	95.1%	5.3	9/2/2026	48	0	18.4	09/02/2026 23:00	172	0
H_2S	ppb	1.8	95.1%	3.0	9/5/2026	3.6	0	8.7	09/01/2026 20:00	11	0
$PM_{2.5}$	µg/m^3	12.2	10.6%	13.3	9/24/2026	28	0	54.5	09/23/2026 23:00	-	-


SAAQS: Saskatchewan Ambient Air Quality Standards

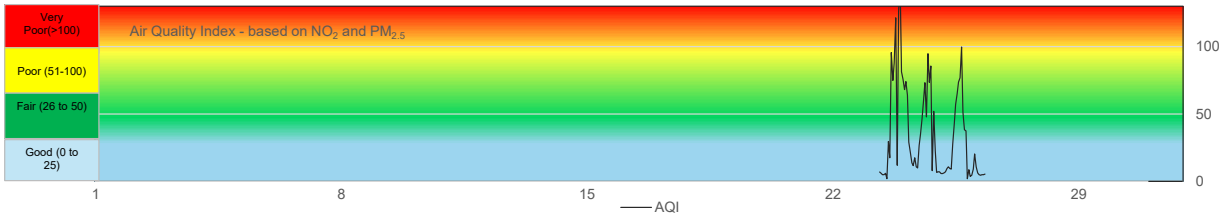



*If AQI cannot be calculated due to missing parameters, AQHI plus is reported using $PM_{2.5}$

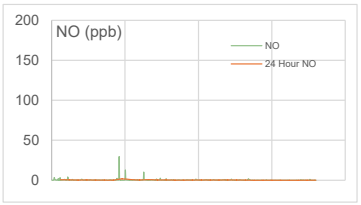


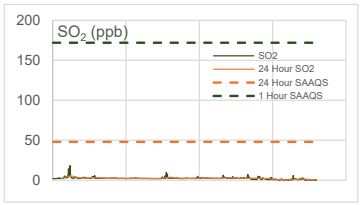


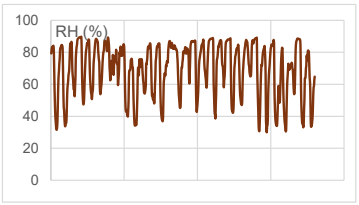


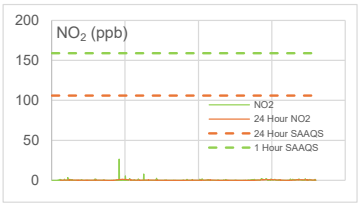

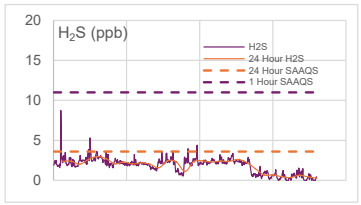

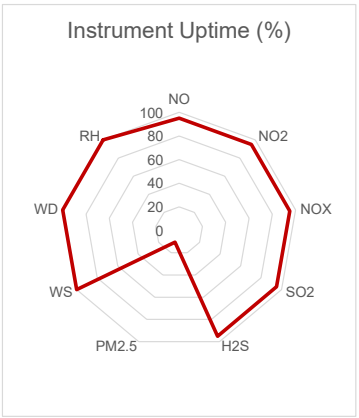

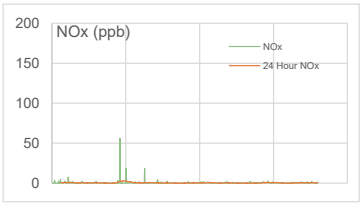


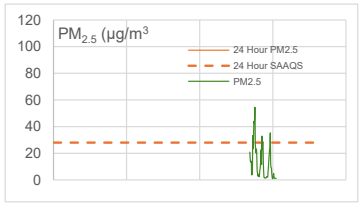


SESAA Weyburn Station - September 2026 Summary Report

Exceedance Summary (24-Hours Average)										
24-hours Exceedance Information			Summary of other Parameters during Exceedance							
Pollutant	Date	Conc.	WS	WD	H_2S	NO	NO_2	NOx	SO_2	$PM_{2.5}$


Exceedance Summary (1-Hour Average)								
1-hour Exceedance Information			Summary of Other Parameters During Exceedance					
Pollutant	Date and Time	Conc.	WS	WD	Precip.	SO_2	NO_2	$PM_{2.5}$

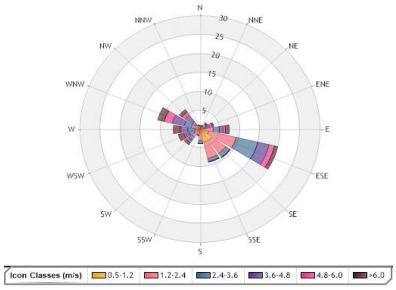


Wind Rose

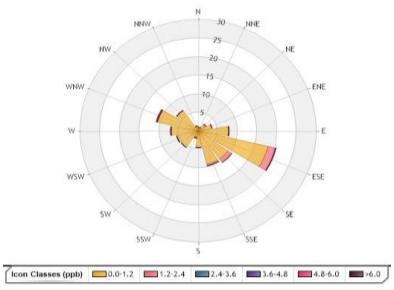


NO_2 Pollution Rose

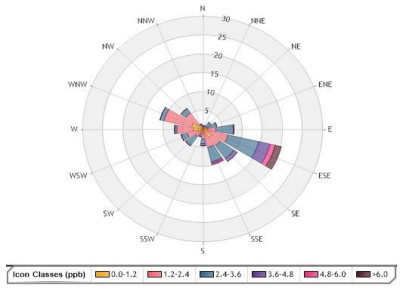

SO_2 Pollution Rose

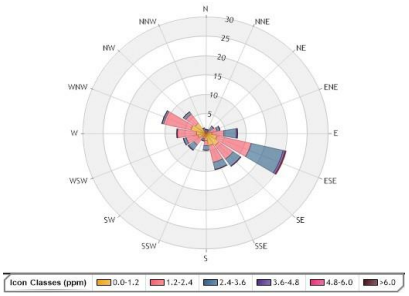

H_2S Pollution Rose

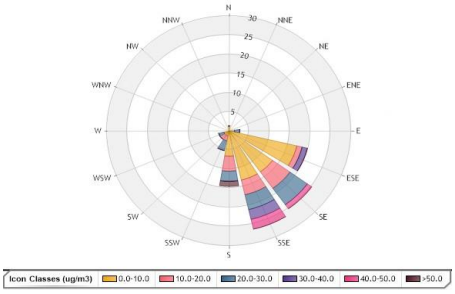

$PM_{2.5}$ Pollution Rose

Parameters	Unit	Color Code for Wind Speed and Pollutant Concentration Class					
Wind Speed	m/s	0.5-W-1.2	1.2-W-2.4	2.4-W-3.6	3.6-W-4.8	4.8-W-6.0	W > 6.0
NO_2	ppb	0.0-C-1.2	1.2-C-2.4	2.4-C-3.6	3.6-C-4.8	4.8-C-6.0	C > 6.0
SO_2	ppb	0.0-C-1.2	1.2-C-2.4	2.4-C-3.6	3.6-C-4.8	4.8-C-6.0	C > 6.0
H_2S	ppb	0.0-C-1.2	1.2-C-2.4	2.4-C-3.6	3.6-C-4.8	4.8-C-6.0	C > 6.0
$PM_{2.5}$	µg/m^3	0.0-C-10.0	10.0-C-20.0	20.0-C-30.0	30.0-C-40.0	40.0-C-50.0	C > 60.0

Monthly Update

* All data has been zero drift and baseline corrected, where required. Data may change after final validation process.
* All compliance parameters were within the Saskatchewan Ambient Air Quality Standards.
* All compliance parameters were more than 90% operational for the month with the exception of $PM_{2.5}$.
* A total of 659 hours of $PM_{2.5}$ data was flagged as "analyzer error," resulting in missing and flatlined data.
* One hour of data were flagged for all gas analyzers due to daily IZS checks, resulting in the loss of one hour of data each day.
* Most recent quarterly calibrations were completed on September 23, 2026.